

PRODUCT MONOGRAPH

HUMALOG[®]

(insulin lispro injection)

Solution for Injection, 100 units/mL, Lilly Standard

ATC Code: A10AB04

fast-acting

HUMALOG[®] 200 units/mL KwikPen[®]

(insulin lispro injection)

Solution for Injection, 200 units/mL, Lilly Standard

ATC Code: A10AB04

fast-acting

HUMALOG[®] MIX25[®]

(25% insulin lispro injection, 75% insulin lispro protamine suspension)

Suspension for Injection, 100 units/mL, Lilly Standard

ATC Code: A10AD04

intermediate- or long-acting combined with fast-acting

HUMALOG MIX50[®]

(50% insulin lispro injection, 50% insulin lispro protamine suspension)

Suspension for Injection, 100 units/mL, Lilly Standard

ATC Code: A10AD04

intermediate- or long-acting combined with fast-acting

THERAPEUTIC CLASSIFICATION

Anti-Diabetic Agent

©Eli Lilly Canada Inc.
Exchange Tower
130 King Street West, Suite 900
P.O. Box 73
Toronto, Ontario
M5X 1B1

Date of Initial Approval:
October 8, 1996

Date of Revision:
April 12, 2021

Submission Control No: 245846

Table of Contents

PART I: HEALTH PROFESSIONAL INFORMATION	3
SUMMARY PRODUCT INFORMATION.....	3
INDICATIONS AND CLINICAL USE.....	3
CONTRAINDICATIONS.....	4
WARNINGS AND PRECAUTIONS.....	5
ADVERSE REACTIONS.....	11
DRUG INTERACTIONS.....	12
DOSAGE AND ADMINISTRATION	13
OVERDOSAGE	15
ACTION AND CLINICAL PHARMACOLOGY.....	16
STORAGE AND STABILITY	20
DOSAGE FORMS, COMPOSITION AND PACKAGING	20
PART II: SCIENTIFIC INFORMATION.....	22
PHARMACEUTICAL INFORMATION.....	22
DETAILED PHARMACOLOGY.....	23
TOXICOLOGY	32
REFERENCES	35
PART III: CONSUMER INFORMATION.....	39

HUMALOG[®]
 (insulin lispro injection)
 Solution for Injection, 100 units/mL, Lilly Standard

HUMALOG[®] 200 units/mL KwikPen[®]
 (insulin lispro injection)
 Solution for Injection, 200 units/mL, Lilly Standard

HUMALOG[®] MIX25[®]
 (25% insulin lispro injection, 75% insulin lispro protamine suspension)
 Suspension for Injection, 100 units/mL, Lilly Standard

HUMALOG MIX50[®]
 (50% insulin lispro injection, 50% insulin lispro protamine suspension)
 Suspension for Injection, 100 units/mL, Lilly Standard

PART I: HEALTH PROFESSIONAL INFORMATION

SUMMARY PRODUCT INFORMATION

Route of Administration	Dosage Form / Strength	Nonmedicinal Ingredients
Parenteral	Solution for Injection, 100 units/mL	HUMALOG (100 units/mL): Dibasic sodium phosphate, glycerol, hydrochloric acid, <i>m</i> -cresol distilled, sodium hydroxide and water for injection, zinc (as ion).
	Solution for Injection, 200 units/mL	HUMALOG (200 units/mL): Glycerol, tromethamine, <i>m</i> -cresol, zinc oxide, water for injection, hydrochloric acid and sodium hydroxide.
	Suspension for Injection, 100 units/mL	HUMALOG MIX25 and HUMALOG MIX50 also contain liquefied phenol, protamine sulphate, and zinc oxide.

INDICATIONS AND CLINICAL USE

HUMALOG (insulin lispro injection), HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension), and HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension) are indicated for the treatment of patients with diabetes mellitus who require insulin for the maintenance of normal glucose homeostasis. HUMALOG insulins are also indicated for the initial stabilization of diabetes mellitus. HUMALOG (insulin lispro injection) is a fast-acting insulin analogue and is for use in conjunction with a longer

acting insulin, such as HUMULIN N (insulin isophane (rDNA origin) NPH), except when used in a subcutaneous insulin infusion pump.

HUMALOG 200 units/mL KwikPen (insulin lispro injection) is reserved for the treatment of patients with diabetes requiring daily doses of more than 20 units of fast-acting insulin.

CONTRAINDICATIONS

The HUMALOG (insulin lispro) family of insulins are contraindicated during episodes of hypoglycemia (see SYMPTOMS AND TREATMENT OF OVERDOSAGE) and in patients sensitive to insulin lispro or any of the excipients they contain (for a complete list of excipients, see DOSAGE FORMS, COMPOSITION AND PACKAGING).

WARNINGS AND PRECAUTIONS

Serious Warnings and Precautions

- Hypoglycemia is the most common adverse effect associated with insulins, including the HUMALOG family of insulins. As with all insulins, the timing of hypoglycemia may differ among various insulin formulations. Glucose monitoring is recommended for all patients with diabetes. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma or even death (see OVERDOSAGE).
- Due to their quick onset of action, the HUMALOG (insulin lispro) family of insulins should be given within 15 minutes before a meal.
- When necessary, HUMALOG (insulin lispro injection) may be given shortly after a meal instead (within 20 minutes of the start of the meal).
- HUMALOG 200 units/mL should not be administered via a subcutaneous infusion pump, or mixed with any other insulin (including HUMALOG 100 units/mL).
- Insulin lispro solution in the HUMALOG 200 units/mL KwikPen cannot be transferred from the prefilled pen to other devices, such as a syringe. The markings on the insulin syringe will not measure the dose correctly. Overdose can result causing severe hypoglycemia.
- When used via a subcutaneous insulin infusion pump, HUMALOG (insulin lispro injection) 100 units/mL should not be diluted or mixed with any other insulin. Patients should carefully read and follow the insulin infusion pump manufacturer's instructions and Part III- Consumer Information before use.
- Any change of insulin or human insulin analogue should be made cautiously and only under medical supervision. Changes in purity, strength, brand (manufacturer), type (insulin lispro, regular, NPH, etc.), species (beef, pork, beef-pork, human), and/or method of manufacture (recombinant DNA versus animal source insulin) may result in the need for a change in dosage (see DOSAGE AND ADMINISTRATION).
- HUMALOG shall not be used if it is not water clear and colourless or if it has formed a deposit of solid particles on the wall of the vial or cartridge.
- HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension) and HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension) are white suspensions. They should be administered by subcutaneous injection only and must not be administered intravenously.

General

As with all insulin therapies, the duration of action of HUMALOG may vary in different individuals or in the same individual according to dose, injection site, blood flow, temperature and level of physical activity.

Hypokalemia is among the potential clinical adverse effect associated with the use of all insulin therapies, including HUMALOG. This potential clinical adverse effect may be relevant in patients who are on potassium lowering drugs or losing potassium through other means (e.g. diarrhea).

Stress or concomitant illness, especially infectious and febrile conditions may change insulin requirements. In these instances, patients should contact their physician and carefully control their blood glucose.

To avoid transmission of disease, a cartridge or prefilled syringe should not be used by more than one person.

HUMALOG (insulin lispro injection) had a similar safety profile to HUMULIN R (insulin injection (rDNA origin) Regular) over the course of the clinical studies. HUMALOG has been shown to control glycosylated hemoglobin (HbA1c) levels as effectively as human insulin in comparator studies specifically designed to study meal time therapy without optimization of basal insulin regimens. Once a patient is using HUMALOG, reassessment and adjustment, as necessary, of the basal insulin regimen (dosage and number of injections) has been shown to optimize overall glycemic control.

Any fast-acting insulin formulation should be used with caution in patients with gastroparesis. However, some patients with gastroparesis may benefit from postprandial administration of HUMALOG, which has been shown to provide postprandial glycemic control similar to that provided by human insulin injected 30 minutes pre-prandially. Using the postprandial dosing approach, the insulin dose can be adjusted according to the actual caloric intake and/or the observed rise in blood glucose following a meal.

Insulin plus Thiazolidinediones (TZDs):

TZDs, alone or in combination with other antidiabetic agents (including insulin), can cause heart failure and edema. The combination of insulin with a TZD is not indicated for the treatment of type 2 diabetes mellitus. Please refer to the respective TZD Product Monograph Warnings and Precautions information when the use of these drugs in combination with any insulin, including HUMALOG, HUMALOG MIX25 and HUMALOG MIX50, is contemplated.

Changes in Insulin Regimen/Transferring Patients from Other Insulins:

Patients taking a HUMALOG insulin may require a change in dosage from that used with their usual insulins. If an adjustment is needed, it may occur with the first dose or during the first several weeks or months.

When patients are transferred between different types of insulin products, including animal insulins, the early warning symptoms of hypoglycemia may change or become less pronounced than those experienced with their previous insulin. Transferring a patient to a new type or brand of insulin should be done only under strict medical supervision. Changes in insulin regimen, strength, timing of administration, manufacturer, type (e.g., regular, NPH, or insulin analogs), or method of manufacture (recombinant DNA versus animal source insulin) may affect glycemic control and predispose to hypoglycemia or hyperglycemia. Make any changes to a patient's insulin regimen under close medical supervision with increased frequency of glucose monitoring. Changes in insulin dose or an adjustment in concomitant oral antidiabetic treatment may be needed. If an adjustment is needed, it may be done with the first doses or during the first few weeks or months and under medical supervision (see WARNINGS AND PRECAUTIONS).

Patients whose blood glucose is greatly improved, e.g., by intensified insulin therapy, may lose some or all of the warning symptoms of hyperglycemia and should be advised accordingly. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma, or death.

Carcinogenesis and Mutagenesis

Like human insulin, in one year animal studies insulin lispro did not produce proliferative effects or tumors in organs and tissues when given at very high subcutaneous doses in chronic toxicity tests. In animal studies, there is no evidence of insulin lispro induced fertility impairment.

Endocrine and Metabolism

Hypoglycemia:

Hypoglycemia is the most frequently occurring undesirable effect of insulin therapy including HUMALOG. Severe hypoglycemia can result in temporary or permanent impairment of brain function and death (see ADVERSE REACTIONS).

Hypoglycemia may occur if the insulin dose is too high in relation to the insulin requirement (see OVERDOSAGE).

Hypoglycemic reactions following treatment with insulin products including HUMALOG are mostly mild and easily managed.

Changes in insulin regimen or changes in life style (i.e. diet, exercise/physical activity) may require a change in dosage to avoid hypoglycemia. Omission of a meal or unplanned strenuous physical exercise may lead to hypoglycemia.

Glucose monitoring is recommended for all patients with diabetes mellitus who are also taking HUMALOG (see Monitoring and Laboratory Tests).

The patient's ability to concentrate and react may be impaired as a result of hypoglycemia. This may constitute a risk in situations where these abilities are of special importance (e.g., driving a car or operating machinery) especially in those who have reduced or absent awareness of the warning signs of hypoglycemia or have frequent episodes of hypoglycemia.

Diabetic patients should be instructed to carry a few lumps of sugar, candies or biscuits to prevent the progression of a hypoglycemic reaction, should one occur (see Part III, CONSUMER INFORMATION).

Hypoglycemia can occur regardless of what type of insulin you take and can cause fatigue, sweating, heart palpitations, disturbed behaviour, hunger, convulsions or loss of consciousness. In extreme circumstances, even death can occur without recognizable symptoms. Some people may not recognize when their blood sugar drops low.

In certain cases (e.g., long duration of diabetes mellitus, diabetic nerve disease, intensified diabetes mellitus control, patients with psychiatric illness, elderly patients or use of medications

such as beta blocking agents), the nature and intensity of early warning symptoms of hypoglycemia (pallor, sweating, anxiety, headache, tachycardia, hunger) may change or be less pronounced.

Hyperglycemia:

Inadequate dosing or discontinuation of HUMALOG, especially in type 1 diabetes mellitus, may lead to hyperglycemia and when untreated, hyperglycemic events may eventually lead to diabetic ketoacidosis or coma which are potentially fatal (see ADVERSE REACTIONS). Usually the first symptoms of hyperglycemia develop gradually over a period of hours or days. They include polydipsia; polyuria; nausea; abdominal pain, vomiting; drowsiness; blurred vision, flushed dry skin; loss of appetite, weight loss as well as acetone odour of breath (see ADVERSE REACTIONS).

Ability to concentrate and react may be impaired as a result of hyperglycemia or as a result of hyperglycemia-induced visual impairment. This may constitute a risk in situations where these abilities are of special importance such as driving a car or operating machinery.

Hepatic/Biliary/Pancreatic

Although impaired hepatic function does not affect the absorption or disposition of HUMALOG, careful glucose monitoring and dose adjustments of insulin, including HUMALOG, may be necessary.

Immune

Injection Site and Local Allergic Reactions:

With insulin therapies including HUMALOG, patients may experience redness, swelling, pain, inflammation, or itching at the site of injection (see ADVERSE REACTIONS).

Most of these minor reactions usually resolve in a few days to a few weeks. They may occur if the injection is not properly made (irritants in the skin cleansing agent or poor injection technique), or if the patient is allergic to the insulin or any excipients (see CONTRAINDICATIONS).

Lipodystrophy and Cutaneous Amyloidosis

Subcutaneous administration of insulin products, including HUMALOG can result in lipodystrophy (depression in the skin), lipohypertrophy (enlargement or thickening of tissue), or localized cutaneous amyloidosis (skin lumps). Patients should be advised to consult their doctor if they notice any of these conditions. Continuous rotation of the injection site within a given area may help reduce or prevent these reactions.

Repeated insulin injections into areas of lipodystrophy or localized cutaneous amyloidosis have been reported to result in hyperglycemia; and a sudden change in the injection site (to an unaffected area) has been reported to result in hypoglycemia.

Systemic Allergic Reactions:

Systemic allergic reactions have rarely occurred with insulin treatments, including HUMALOG (see ADVERSE REACTIONS). These reactions may be characterized by a generalized rash (with pruritus), shortness of breath, wheezing, angioneurotic edema and drop in blood pressure (see ADVERSE REACTIONS).

Severe cases of generalized allergy including anaphylactic reaction may be life threatening (see CONTRAINDICATION).

Antibody Production:

Immune responses can occur with insulin products, including production of auto antibodies (IgG). In general, glycemic control is not affected by the presence of auto antibodies. Very rarely, auto antibodies may cause hyperglycemia (insulin resistance) or hypoglycemia (inappropriate release). Insulin antibodies are frequently cross-reactive. Patients who have demonstrated an allergic reaction to other insulin products may demonstrate an allergic reaction to HUMALOG.

Renal

The requirements for insulin may be reduced in patients with renal impairment.

Reproduction Studies

There are no adequate and well-controlled studies with HUMALOG during pregnancy and lactation (see TOXICOLOGY).

Information for Patients

Patients should be informed about potential advantages and disadvantages of HUMALOG therapy, including possible side effects. Patients should also be offered continued education and advice on insulin therapies, delivery device options, life-style management, self-monitoring, complications of insulin therapy, timing of dosage, and instruction for use of injection devices, storage of insulin, travelling and others (see PART III: CONSUMER INFORMATION).

Female patients with diabetes mellitus should be advised to inform their doctor if they are pregnant or are contemplating pregnancy. Careful monitoring of glucose control, as well as general health is essential in pregnant patients with diabetes (see Special Populations and PART III: CONSUMER INFORMATION).

Special Populations

Pregnant Women

HUMALOG can be used in pregnancy if clinically indicated. Data on a large number of exposed pregnancies do not indicate any adverse effect of HUMALOG 100 units/mL on pregnancy or on the health of the foetus/newborn. It is essential to maintain good glucose control in both gestational diabetes and throughout pregnancy in type 1 and type 2 patients. Insulin

requirements usually decrease during the first trimester and increase during the second and third trimesters.

Patients with diabetes should be advised to inform their doctor if they are pregnant or are contemplating pregnancy. Careful monitoring of glucose control, as well as general health is essential in pregnant patients with diabetes. During the perinatal period, careful monitoring of infants born to mothers with diabetes is warranted.

Nursing Women

The use of HUMALOG insulins in nursing mothers has not been studied. Diabetic patients who are nursing may require adjustments in insulin dose and/or diet.

Pediatrics (3 to 18 years of age)

Clinical trials have been performed in children (61 patients aged 3 to 11) and children and adolescents (481 patients aged 9 to 18 years), comparing HUMALOG 100 units/mL to regular human insulin. HUMALOG 100 units/mL showed better postprandial blood glucose control while maintaining a similar safety profile.

As in adults, HUMALOG 100 units/mL should be given within 15 minutes before a meal. When necessary, HUMALOG 100 units/mL may be given shortly after a meal instead (within 20 minutes of the start of the meal).

The safety and effectiveness of HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension) and HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension) in children have not been established.

Geriatrics (> 65 years of age)

HUMALOG may be used in elderly patients, if clinically indicated.

Information on the effect of age and gender on the pharmacokinetics of HUMALOG is unavailable. However, in large clinical trials, sub-group analysis based on age and gender did not indicate any difference in postprandial glucose parameters between HUMALOG 100 units/mL and regular human insulin.

In clinical studies of HUMALOG 100 units/mL, glycosylated hemoglobin (HbA_{1c}) values and hypoglycemia rates in patients \geq 65 years of age did not differ from younger patients. Clinical studies of HUMALOG MIX25 and HUMALOG MIX50 did not include sufficient number of patients \geq 65 years to determine whether they respond differently than younger patients.

In general, dose selection for an elderly patient should take into consideration the greater frequency of decreased hepatic, renal, or cardiac function, and of concomitant disease or other drug therapy in this population.

Other Disease States

Control of diabetes mellitus may be further complicated by diseases such as acromegaly, Cushing's syndrome, hyperthyroidism and pheochromocytoma.

Monitoring and Laboratory Tests

Self-Monitoring of Blood Glucose

With insulin therapy, including HUMALOG, the need for regular blood glucose self-monitoring should be considered to obtain optimal glycemic control (see PART III: CONSUMER INFORMATION). HbA_{1C} should be measured every 3 to 4 months in all patients taking insulin products.

ADVERSE REACTIONS

Body as a Whole – Allergic Reaction(s)

Local allergy in patients may occur as redness, swelling, or itching at the site of injection. These minor reactions usually resolve in a few days to a few weeks. In some instances, these reactions may be related to factors other than insulin, such as irritants in the skin cleansing agent or poor injection technique.

Systemic allergy to insulin is less common but potentially more serious. Generalized allergy to insulin may cause rash over the whole body, shortness of breath, wheezing, reduction in blood pressure, rapid pulse or sweating. Severe cases of generalized allergic reaction may be life-threatening.

Skin and Appendages – injection site reaction, lipodystrophy, pruritis, rash.

Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the skin) or lipohypertrophy (enlargement or thickening of tissue). Patients should be advised to consult their doctor if they notice any of these conditions. A change in injection technique may help alleviate the problem.

Metabolic – Hypoglycemia is the most frequent undesirable effect of insulin therapy that a patient with diabetes may suffer. Severe hypoglycemia may lead to loss of consciousness and, in extreme cases, death.

Continuous Subcutaneous Insulin Infusion – HUMALOG 100 units/mL ONLY

In a 39-week, randomized open-label, three way crossover, controlled multicenter study in patients with type 1 diabetes, the perceived catheter set occlusion rates were similar across fast-acting insulin analog, including HUMALOG, insulin aspart and insulin glulisine (Figure 1).

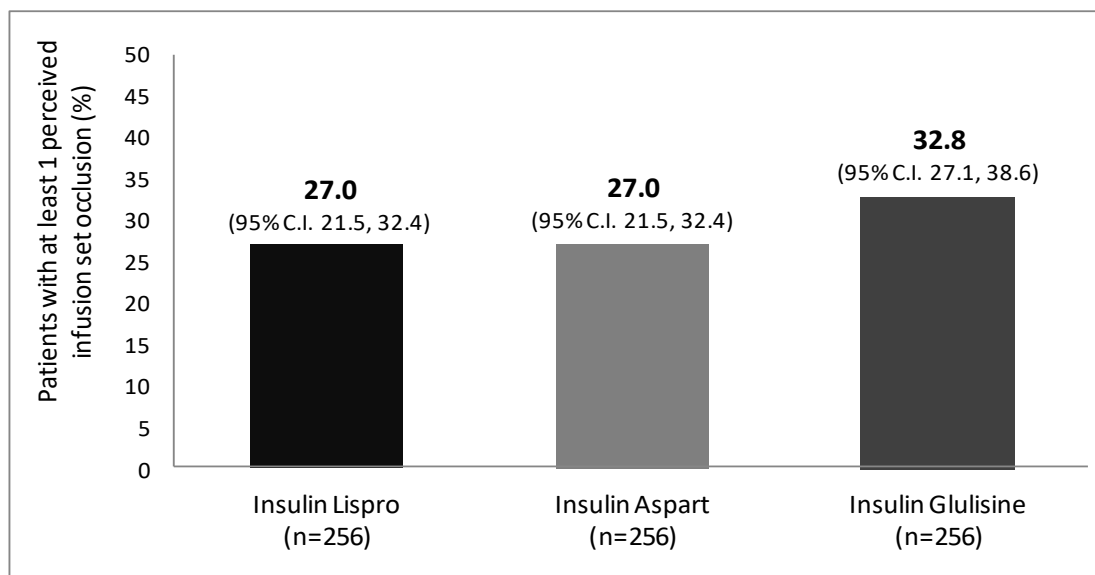


Figure 1. Patients (%) with at least 1 perceived set occlusion over 13 weeks.

In a 12-week, randomized, crossover study in adult patients with type 1 diabetes (n=39), the rates of catheter occlusions and infusion site reactions were similar for HUMALOG 100 units/mL and regular human insulin treated patients (Table 1).

Table 1. Rates of Catheter Occlusions and Infusion Site Reactions

	HUMALOG 100 units/mL (n=38)	Regular Human Insulin 100 units/mL (n=39)
Number of catheter occlusion/month	0.09	0.10
Infusion site reactions	2.6% (1/38)	2.6% (1/39)

Post-Market Adverse Drug Reactions

Cases of edema have been reported with insulin therapy, including HUMALOG, particularly if previous poor metabolic control is improved by intensified insulin therapy.

DRUG INTERACTIONS

Drug-Drug Interactions

Drug interactions with insulin formulations including HUMALOG insulins may include the following:

Insulin requirements may be decreased in the presence of agents such as oral hypoglycemic agents, octreotide, salicylates, sulfa antibiotics, certain antidepressants (monoamine oxidase inhibitors), non-selective beta-adrenergic blockers, alcohol, angiotensin converting enzyme inhibitors and angiotensin II receptor blockers and anabolic steroids.

Drugs that may increase insulin requirements such as oral contraceptives, thiazides, glucocorticosteroids, thyroid hormones, sympathomimetics, and danazol. The hypoglycemic action of insulin may also be antagonized by diphenylhydantoin.

Hormones that tend to counteract the hypoglycemic effects of insulin include growth hormone, corticotropin, glucocorticoids, thyroid hormone, and glucagon. Epinephrine not only inhibits the secretion of insulin, but also stimulates glycogen breakdown to glucose. Thus, the presence of such diseases as acromegaly, Cushing's syndrome, hyperthyroidism, and pheochromocytoma complicate the control of diabetes.

Insulin requirements can be increased, decreased, or unchanged in patients receiving diuretics.

To avoid the risk of developing new or worsening heart failure, the use of TZDs in combination therapy with insulin is not indicated (see WARNINGS AND PRECAUTIONS).

The physician should be consulted when using other medications in addition to HUMALOG.

Drug-Lifestyle Interactions

Hypoglycemia may occur as a result of an excess of insulin relative to food intake, energy expenditure, or both. Omission of a meal or unplanned strenuous physical exercise may lead to hypoglycemia (see WARNINGS AND PRECAUTIONS, and OVERDOSAGE).

DOSAGE AND ADMINISTRATION

Dosing Considerations

The dosage of HUMALOG, HUMALOG MIX25, or HUMALOG MIX50 is determined by a physician in accordance with the requirements of the patient.

Although HUMALOG insulins have a quicker onset of action and shorter duration of activity, dosing is comparable to regular human insulin. The dosage of a HUMALOG insulin, like all other insulin formulations, is dependent upon the individual patient requirements. The dose and number of insulin injections should be adjusted to maintain blood glucose concentrations as close to normal as possible.

Additional adjustment of dosage may be required in diabetes patients with renal impairment, during intercurrent illness and/or emotional disturbances.

Adjustment of dosage may also be necessary if patients undertake increased physical activity or change their usual diet.

Recommended Dose and Dosage Adjustment

New Patients:

Patients receiving insulin for the first time can be started on a HUMALOG insulin in the same manner as they would be on animal-source or human insulin.

Patients should be monitored closely during the adjustment period.

Transfer Patients:

When transferring patients to a HUMALOG insulin, use the same dose and dosage schedule. However, some patients transferring to a HUMALOG insulin may require a change in dosage from that used with their previous insulin. Analysis of a database of type 1 diabetic patients indicated that basal insulin requirements increased by 0.04 U/Kg, while HUMALOG requirements decreased by 0.03 U/Kg, after one year of treatment. For type 2 diabetic patients, both fast acting and basal insulin requirements increased slightly after one year of treatment with both HUMALOG and HUMULIN R.

Optimizing Glycemic Control:

In order to achieve optimal glycemic control, changes in total daily dosage, the number of injections per day, and/or timing of injections may be necessary when using a HUMALOG insulin.

Once a patient is using HUMALOG, reassessment and adjustment as necessary of the basal insulin regimen (dosage and number of injections) has been shown to optimize overall glycemic control.

Administration

HUMALOG is a clear, colourless solution. It is important to always examine the appearance of the vial or cartridge of HUMALOG prior to administration. It should not be used if it is cloudy, unusually viscous or gelled, precipitated, or even slightly coloured; if there are clumps floating in the liquid, or if particles appear to be sticking to the sides or bottom of the vial or cartridge.

HUMALOG 100 units/mL should be given by subcutaneous injection or by continuous subcutaneous insulin infusion pump and may, although not recommended, also be given by intramuscular injection. When administered by continuous subcutaneous infusion by an external insulin pump, the HUMALOG in the reservoir should be changed at least every 14 days. Infusion sets should be changed according to pump manufacturer's instructions (typically 3 days is recommended) or as directed by healthcare professionals. It may also be administered intravenously under conditions where regular human insulin is given intravenously. When used as a meal-time insulin, HUMALOG should be given within 15 minutes before a meal, or when necessary shortly after a meal instead (within 20 minutes of the start of the meal).

HUMALOG 200 units/mL is given by subcutaneous injection and should be reserved for the treatment of patients with diabetes requiring daily doses of more than 20 units of fast-acting insulin. HUMALOG 200 units/mL should not be withdrawn from the prefilled insulin device or mixed with any other insulin (see Warnings and Precautions). HUMALOG 200 units/mL should not be administered intravenously or by subcutaneous infusion pump as these methods of administration have not been studied.

HUMALOG MIX25 and HUMALOG MIX50 are white suspensions. They should be administered by subcutaneous injection only and must not be administered intravenously.

HUMALOG MIX25 and HUMALOG MIX50 start lowering blood glucose more quickly than regular human insulin, and should be given within 15 minutes before a meal.

Subcutaneous administration, preferably by the patient, should be in the upper arms, thighs, buttocks or abdomen. Injection sites should be rotated so that the same site is not used more than approximately once a month, in order to reduce the risk of lipodystrophy and localized cutaneous amyloidosis. Do not inject into areas of lipodystrophy or localized cutaneous amyloidosis. When compared to HUMULIN R, HUMALOG retains its more rapid onset and shorter duration of action irrespective of the subcutaneous injection site used.

Care should be taken to ensure that a blood vessel has not been entered. The injection site should not be massaged.

Instructions for Use/Handling

To prevent the possible transmission of disease, never share a HUMALOG, HUMALOG 200 units/mL, HUMALOG MIX25, HUMALOG MIX50 pen or cartridge between patients, even if the needle on the delivery device is changed.

Mixing of Insulins:

Mixing HUMALOG 100 units/mL with HUMULIN N does not decrease the absorption rate or the total bioavailability of HUMALOG. Given alone or mixed with HUMULIN N, HUMALOG results in a more rapid absorption and glucose-lowering effect compared with human regular insulin.

If HUMALOG 100 units/mL is mixed with a long-acting insulin, HUMALOG 100 units/mL should be drawn into the syringe first to prevent clouding of the HUMALOG 100 units/mL by the long-acting insulin. Injection should be made immediately after mixing. Mixtures should not be administered intravenously. HUMALOG 100 units/mL should not be diluted or mixed with any other insulin when used in a subcutaneous insulin infusion pump.

HUMALOG 200 units/mL should not be mixed with any other insulin.

The effects of mixing HUMALOG, HUMALOG MIX25, or HUMALOG MIX50 with either animal-source insulins or human insulin preparations produced by other manufacturers have not been studied. This practice is not recommended.

OVERDOSAGE

With the rapid onset of activity of the HUMALOG family of insulins, it is important that the insulin analogue be given close to mealtime (within 15 minutes before a meal). When necessary, HUMALOG may be given shortly after a meal instead (within 20 minutes of the start of the meal). A significant deviation could put the patient at risk of hypoglycemia.

Insulins have no specific overdose definitions because serum glucose concentrations are a result of complex interactions between insulin levels, glucose availability and other metabolic processes. Hypoglycemia may occur as a result of an excess of insulin or HUMALOG relative

to food intake and energy expenditure or in patients who have an infection or become ill (especially with diarrhea or vomiting).

Hypoglycemia may be associated with listlessness, confusion, palpitations, headache, sweating and vomiting.

Mild hypoglycemic episodes will respond to oral administration of glucose or sugar-containing foods.

Correction of moderately severe hypoglycemia can be accomplished by intramuscular or subcutaneous administration of glucagon, followed by oral carbohydrate when the patient recovers sufficiently. Patients who fail to respond to glucagon must be given glucose solution intravenously.

Patients who are unable to take sugar orally or who are unconscious should be treated with intravenous administration of glucose at a medical facility or should be given an injection of glucagon (either intramuscular or subcutaneous). The patient should be given oral carbohydrates as soon as consciousness is recovered.

For management of a suspected drug overdose, contact your regional Poison Control Centre.

ACTION AND CLINICAL PHARMACOLOGY

Mechanism of Action

Insulin lispro, the active pharmaceutical ingredient in HUMALOG 100 units/mL, HUMALOG 200 units/mL, HUMALOG MIX25, and HUMALOG MIX50 is created by inverting the natural Pro-Lys sequence in human insulin at positions 28 and 29 in the C terminal portion of the B-chain. This change in amino acid sequence slightly modifies the physicochemical properties of the molecule relative to native human insulin in such a manner that insulin lispro self-associates less avidly and dissociates into its monomeric form more rapidly than regular insulin. As a result, insulin lispro is absorbed more rapidly than regular soluble insulin from subcutaneous sites of injection and also has a shorter duration of action.

The reversed sequence of lysine and proline in insulin lispro, is identical to that on the B-chain of human IGF-1. The incidence of self-association with IGF-1 is known to be lower than observed with human insulin. Incorporating this IGF-1-like feature into the human insulin molecule markedly changes the physico-chemical behaviour of the resulting insulin lispro but does not significantly alter its pharmacodynamic action because the terminal part of the B-chain does not participate in insulin's interaction with the insulin receptor. In vitro experiments showed that insulin lispro interacts with the insulin receptor much like regular human insulin does. Although binding to the IGF-1 receptor is higher than for regular human insulin (1.5 times more) it is significantly less than that of IGF-1 itself (more than a thousand times less) and does not promote cell growth in biological assays to any greater extent than human insulin.

The primary activity of insulins, including HUMALOG, HUMALOG MIX25, and HUMALOG MIX50, is the regulation of glucose metabolism. In addition, all insulins have several anabolic

and anti-catabolic actions on many tissues in the body. In muscle and other tissues (except the brain), insulin causes rapid transport of glucose and amino acids intracellularly, promotes anabolism, and inhibits protein catabolism. In the liver, insulin promotes the uptake and storage of glucose in the form of glycogen, inhibits gluconeogenesis and promotes the conversion of excess glucose into fat.

Pharmacodynamics and Pharmacokinetics

HUMALOG 100 units/mL

HUMALOG is absorbed more rapidly than regular soluble insulin from subcutaneous sites of injection and also has a shorter duration of action. Due to its quick onset of action, HUMALOG should be given within 15 minutes before a meal. When necessary, HUMALOG may be given shortly after a meal instead (within 20 minutes of the start of the meal). The duration of action of HUMALOG 100 units/mL and 200 units/mL is between 3.5 and 4.75 hours.

Subcutaneously injected regular insulin typically results in serum insulin concentrations that peak later and remain elevated for a longer time than those following normal pancreatic insulin secretion in non-diabetics. When regular insulin is used to control postprandial blood glucose, adequate control is often not achieved because the amount of regular insulin needed to normalize postprandial glucose excursion often leads to late hypoglycemia. By producing more rapid and higher serum insulin concentrations with a shorter duration of activity, HUMALOG decreases glucose excursion during and after meals with less chance for hypoglycemia.

A glucose clamp study was performed, in healthy volunteers, in which a 10 Unit dose of HUMALOG 100 units/mL was compared to HUMULIN R. Doses were given subcutaneously; an additional 10 Unit dose of intravenous regular insulin was given as an absolute reference.

HUMALOG 100 units/mL showed statistically higher peak concentrations (C_{max}) which occurred earlier than observed with HUMULIN R (t_{max}). Total absorption was comparable, with area under the curve (AUC) values of serum concentration vs. time which were not statistically different (Tables 2, 3).

Table 2. Pharmacodynamics of HUMALOG 100 units/mL Compared with HUMULIN R 100 units/mL in Healthy Volunteers.

Mean	HUMALOG 100 units/mL	HUMULIN R 100 units/mL
Duration of action (hr)*	3.5-4.75 hr	5.0-7.5 hr
Onset of Action (hr)*	0.5-0.75 hr	0.5-1.0 hr
Time of Maximum Effect (hr)*	0.75-2.5 hr	0.75-4.5 hr

*Results predicted from a pharmacokinetic-pharmacodynamic link model

Table 3. Pharmacokinetics of HUMALOG 100 units/mL Compared with HUMULIN R 100 units/mL in Healthy Volunteers.

Mean	HUMALOG 100 units/mL	HUMULIN R 100 units/mL
t_{max} (min)	53 ± 30	101 ± 40
C_{max} (ng/mL)	3.20 ± 1.33	1.79 ± 0.77
AUC (ng•min/mL)	380 ± 52.2	423 ± 71.8

Subsequent pharmacokinetic studies in type 1 patients confirmed that a significantly faster increase in serum insulin levels and a shorter plasma half life resulted from an injection of HUMALOG 100 units/mL when compared to HUMULIN R (Figure 2).

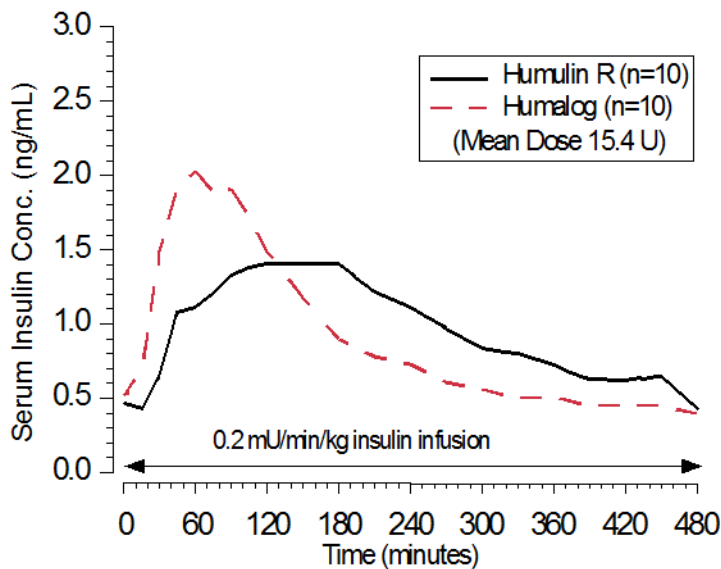


Figure 2. Mean Serum Insulin Concentrations in type 1 Patients Following Injection of HUMULIN R and HUMALOG 100 units/mL (Basal 0.2mU/min/kg insulin infusion).

Postprandial and overall glycemic control: In clinical studies after one year, the decrease in glucose excursion during and after meals with HUMALOG 100 units/mL was consistent, although not always significant, when compared to HUMULIN R. However, there was no significant difference in HbA_{1c} levels between the two treatment groups. These studies were specifically designed to study meal time therapy without optimization of basal insulin regimens.

Subsequent clinical studies have demonstrated that in an intensive insulin treatment regimen with basal insulin optimization, HUMALOG 100 units/mL controls postprandial glucose and contributes to lower HbA_{1c} levels to a greater degree than regular human insulin, without increasing the risk of hypoglycemia.

Hypoglycemia: The frequency of hypoglycemia was not statistically significant in one year parallel studies (HUMALOG 100 units/mL, n=543; HUMULIN R, n=561), but was significantly less with HUMALOG therapy in a six month crossover study in type 1 patients (n=1008) which also demonstrated a significant reduction in nocturnal hypoglycemia with HUMALOG.

Use in Pumps:

When used in subcutaneous insulin infusion pumps, treatment with HUMALOG 100 units/mL has been shown to result in lower HbA_{1c} levels compared to regular human insulin without increasing the risk of hypoglycemia. In clinical trials that compared HUMALOG 100 units/mL with regular human insulin, HUMALOG 100 units/mL consistently showed significant HbA_{1c} improvement in the range of 0.33% to 0.65%.

Hepatic Insufficiency:

Some studies with human insulin have shown increased circulating levels of insulin in patients with hepatic failure. In a study of 22 patients with type 2 diabetes, impaired hepatic function did not affect the subcutaneous absorption or general disposition of HUMALOG when compared to patients with no history of hepatic dysfunction. In that study, HUMALOG maintained its more rapid absorption and elimination when compared to human regular insulin. Careful glucose monitoring and dose adjustments of insulin, including HUMALOG, may be necessary in patients with hepatic dysfunction.

Renal Insufficiency:

Some studies with human insulin have shown increased circulating levels of insulin in patients with renal failure. In a study of 25 patients with type 2 diabetes and varying degrees of renal function (from normal to severe impairment, including endstage renal failure), the pharmacokinetic differences between HUMALOG and human regular insulin were generally maintained. However, the sensitivity of the patients to insulin did change, with an increased response to insulin as the renal function declined. Careful glucose monitoring and dose adjustments of insulin, including HUMALOG, may be necessary in patients with renal dysfunction.

HUMALOG MIX25 AND HUMALOG MIX50:

Insulin lispro protamine suspension (NPL) is a fast-acting and intermediate-acting protamine formulation of insulin lispro that displays absorption and activity profiles similar to those of HUMULIN N (insulin isophane). Fixed mixtures of insulin lispro injection and insulin lispro protamine suspension provide the fast-acting blood glucose lowering activity associated with insulin lispro injection in combination with the intermediate-acting blood glucose lowering activity associated with the insulin lispro protamine suspension.

The HUMALOG family of insulins includes fixed mixtures of insulin lispro injection and insulin lispro protamine suspension that have been formulated in ratios of 25% insulin lispro injection, 75% insulin lispro protamine suspension (HUMALOG MIX25) and 50% insulin lispro injection, 50% insulin lispro protamine suspension (HUMALOG MIX50). The pharmacokinetic and pharmacodynamic profiles of various fixed mixtures were investigated in a glucose clamp study. The rapid activity of insulin lispro was maintained within each mixture. In addition, each

mixture demonstrated a distinct pharmacokinetic and glucodynamic profile. The duration of action of HUMALOG MIX25 and HUMALOG MIX50 is up to 22 hours.

STORAGE AND STABILITY

Prior to first use, HUMALOG preparations must be stored in a refrigerator between 2° and 8°C. They should not be frozen or exposed to excessive heat or sunlight. Cartridges, vials, and prefilled pens that are in current use, should be stored at room temperature (below 30°C and away from direct heat and light) and discarded after 28 days. Do not use after expiry date on label.

When administered by continuous subcutaneous infusion by an external insulin pump, the HUMALOG 100 units/mL in the reservoir should be changed at least every 14 days. Infusion sets should be changed according to pump manufacturer's instructions (typically 3 days is recommended) or as directed by healthcare professionals.

DOSAGE FORMS, COMPOSITION AND PACKAGING

HUMALOG (insulin lispro injection) 100 units/mL is available as a clear, colourless, aqueous solution for parenteral administration in vials, cartridges or prefilled insulin delivery devices:

- Vial, 10 mL
- Vial, 3 mL,
- Cartridge, 3 mL, 5 cartridges/box
- KwikPen, 3 mL prefilled pen, 5 pens/box
- Junior KwikPen; 3 mL prefilled pen, 5 pens/box

HUMALOG (insulin lispro injection) 200 units/mL is available as a clear, colourless, aqueous solution for parenteral administration in a prefilled insulin delivery device:

- KwikPen, 3 mL prefilled pen, 5 pens/box
- KwikPen, 3 mL prefilled pen, 2 pens/box

HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension) is available as a white suspension for parenteral administration in cartridges or prefilled insulin delivery devices:

- Cartridge, 3 mL, 5 cartridges/box
- KwikPen, 3 mL prefilled pen, 5 pens/box

HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension) is available as a white suspension for parenteral administration in cartridges or prefilled insulin delivery devices:

- Cartridge, 3 mL, 5 cartridges/box
- KwikPen, 3 mL prefilled pen, 5 pens/box

Not all pack sizes and presentations may be marketed.

Cartridges are designed for use with Lilly injector systems. The cartridge containing HUMALOG 100 units/mL, HUMALOG MIX25, or HUMALOG MIX50 is not designed to allow any other insulin to be mixed in the cartridge or for the cartridge to be reused.

Non-medicinal Ingredients:

HUMALOG 100 units/mL contains glycerol, dibasic sodium phosphate, *m*-cresol, zinc (as ion) and water for injection. Hydrochloric acid or sodium hydroxide may be added to adjust pH.

HUMALOG MIX25 and HUMALOG MIX50 also contain liquefied phenol, protamine sulphate, and zinc oxide.

HUMALOG 200 units/mL contains glycerol, tromethamine, *m*-cresol, zinc oxide, hydrochloric acid and sodium hydroxide (for pH adjustment) and water for injection.

PART II: SCIENTIFIC INFORMATION

PHARMACEUTICAL INFORMATION

Drug Substance


Proper name: Insulin lispro

Chemical name: Lys(B28), Pro(B29) Human Insulin Analogue
(recombinant DNA origin)

Molecular formula: $C_{257}H_{383}N_{65}O_{77}S_6$

Molecular mass: Molecular Weight: 5808

Structural formula: Insulin lispro is identical in structure to human insulin except for amino acids 28 and 29 of the B-chain; the analogue is Lys(B28) Pro(B29) whereas human insulin is Pro(B28) Lys(B29).

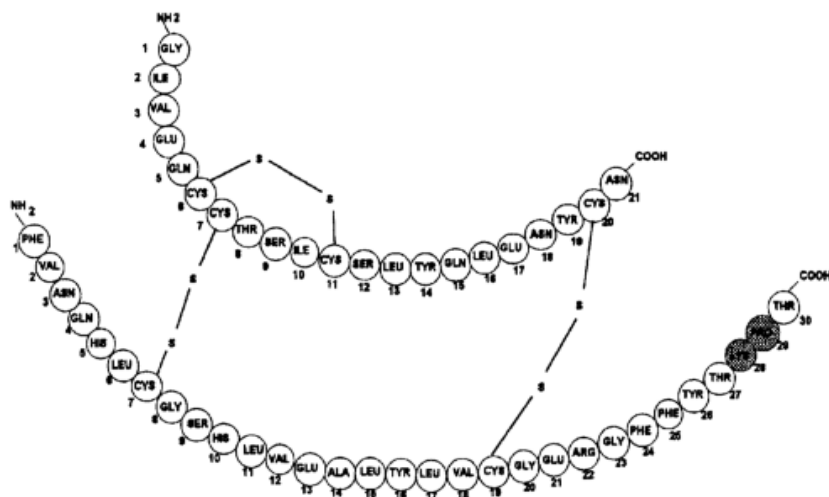

Description: Zinc-insulin lispro crystals appear as a white to off-white solid

Solubility Profile Soluble in:
0.01 M Hydrochloric acid
0.2 M Sodium sulfate, pH 2.3
0.2 M Sodium phosphate, pH 2.2
0.4 M Ammonium bicarbonate, pH 7.5

pI: Approximately 5.65

DETAILED PHARMACOLOGY

The absorption of insulin is dependent on the disassociation of insulin hexamers, which form when insulin is prepared at concentrations found in commercial insulin preparations. The formation of the hexamers occurs by self-association of insulin molecules at the C-terminal end of the B chain. IGF-1 contains an area which shares some homology with human insulin.

Previous studies demonstrated that IGF-1 does not form hexamers. It was also noted that in the area of IGF-1 which is analogous to the 28 and 29 position of the B chain for human insulin, the amino acid sequence is lysine proline, the reverse of the human insulin sequence. The development of HUMALOG (insulin lispro) insulins is based on the reversal of these two amino acids in human insulin.

In the absence of excipients, insulin lispro shows little tendency to self-association. Unlike soluble insulin, insulin lispro will not form hexamers, or crystals, except in the presence of zinc or phenol or *m*-cresol. The latter are widely used preservatives in pharmaceutical insulin preparations. Thus, a unique mechanism is provided whereby formulations of insulin lispro are stabilized against physical and chemical degradation, yet dissociate more rapidly than traditional insulin preparations following injection.

Insulin lispro dissociates into monomers almost immediately in dilute solution, due to rapid loss of phenol or *m*-cresol from the insulin-zinc complexes. A similar phenomenon is assumed to occur following subcutaneous injection. It can be noted that addition of zinc and *m*-cresol, to insulin lispro preparations does result in slightly slower absorption, as compared to a solution prepared from pure insulin lispro crystals, although formulated insulin lispro still absorbs faster than soluble regular insulin preparations and retains its glucodynamic advantages.

Preclinical Pharmacology

The minor amino acid sequence inversion in insulin lispro does not significantly affect the biological properties of insulin lispro as described below. *In vivo* studies were conducted with rats, rabbits, dogs and two different pig models. These studies demonstrated that insulin lispro is equivalent to human insulin with respect to hypoglycemic potency. The dog study and one of the pig studies also showed very convincingly that insulin lispro is more rapidly absorbed from subcutaneous injection sites.

In Vitro Studies:

Insulin lispro was compared to human insulin and found to be equipotent in terms of binding to the human placental insulin receptor and in stimulating [¹⁴C]glucose uptake into rat adipocytes. Insulin lispro has been shown to have a slightly higher affinity to the human placental and skeletal muscle IGF-1 receptors than human insulin (approximately 1.5 times). However, both insulin lispro and human insulin have affinities that are approximately 0.001 times that of IGF-1 itself.

In one study, insulin lispro was found to be approximately 2 times more potent than human insulin at stimulating [³H]thymidine incorporation into human aortic smooth muscle cells (a measure of cellular proliferation), while in another study insulin lispro and human insulin were

equipotent at stimulating growth of human mammary epithelial cells (ED_{50} insulin, 16.0 ± 3.0 nM; ED_{50} insulin lispro, 18.6 ± 4.0 nM, $n=4$, $p=NS$).

In Vivo Studies:

Rat Hypoglycemia Test: Studies with normal male rats indicated that the effective dose needed to give a 50% hypoglycemic response ($ED_{50} \pm SEM$) was 7.2 ± 0.3 $\mu\text{g/kg}$ for insulin lispro and 7.8 ± 0.1 $\mu\text{g/kg}$ for human insulin. In this study the analogue was 108% as active as human insulin, no difference in time of action was found.

Rabbit Hypoglycemia Test: A modified British Prolongation test was conducted using 95 rabbits to compare insulin lispro with U 40 HUMULIN R. Insulin lispro was also formulated at 40 U/mL assuming full potency (i.e., 28.85 U/mg protein). Blood samples were collected at 20, 40, 60, 90, 120, 150, and 210 minutes following subcutaneous injections of each insulin (0.2 U/kg). Resulting blood glucose profiles were virtually identical with the exception of a significantly lower glucose level at 20 minutes for insulin lispro.

Experiments in Dogs: Several dose ranging and time action experiments were conducted in dogs comparing insulin lispro with various human insulin formulations. An optimal experimental design involved the subcutaneous administration of 0.1 U/kg for both the insulin lispro and HUMULIN R (both insulins formulated at 100 U/mL). Blood glucose levels decreased faster and returned to normal sooner in the dogs treated with the insulin lispro. Likewise, the serum levels of the compound rose more rapidly than the human insulin levels.

Studies in Pigs: Crossbred barrows weighing 60 to 85 kg were given subcutaneous injections of either insulin lispro or HUMULIN R, each formulated at 20 U/mL. This animal model was very sensitive to both insulins with 0.1 U/kg causing up to a 75% reduction in blood glucose. A dose of 0.025 U/kg caused a 23% fall in blood glucose for both insulins with evidence for a quicker action with insulin lispro.

The kinetics of insulin lispro was compared to HUMULIN R in 12 pigs with surgically pre-implanted jugular venous and arterial catheters. Twenty hour-fasted animals underwent two studies: (i) an IV injection and (ii) a subcutaneous injection (300 mU/kg) of insulin or analogue. Insulin kinetics over the range of concentrations studied were assumed linear and absorption rates of the insulin and analogues were calculated by deconvolution of their levels after subcutaneous injection with the corresponding IV decay curve. Normoglycemia was maintained by glucose infusion using a glucose controller. The time course of absorption was as follows: % absorbed for HUMULIN R and lispro respectively, at $t=15$ min were 16 and 17%; $t=30$ min: 30 and 46%; $t=45$ min: 42 and 67%; $t=60$ min: 53 and 78%; $t=90$ min: 70 and 88%; $t=120$ min: 82 and 93%. Thus, HUMULIN R peaks rapidly (15 ± 6 min) but at only $1.2 \pm 0.03\%$ absorption/min and continues to be absorbed over an extended period (170 min for $93 \pm 4\%$ absorption). Insulin lispro peaks at 21 ± 2 min but at $2 \pm 0.02\%$ absorption/min and is almost completely ($93 \pm 3\%$) absorbed by 2 hours.

Cardiovascular, Respiratory, and Renal Effects: Insulin lispro was examined for potential cardiovascular and respiratory effects in male beagle dogs anesthetized with α -chloralose. Animals (3/group) received 0.05 mL vehicle/kg (HUMULIN BR Diluent) or 0.1 U/kg insulin lispro intravenous (IV) bolus injection. Cardiovascular, electrocardiographic, and respiratory

parameters were measured prior to dosing, and at 5, 10, 15, 30, 45, and 60 minutes after dosing. No toxicologically important changes in QRS duration (maximum 9% at 10 min) and Q-Tc interval (maximum 10% at 5 min) occurred. The increases in QRS duration and Q-Tc interval were similar to that observed after administration of 0.1 units/kg of regular human insulin.

Female Fischer 344 rats (8/group) were given a single subcutaneous dose of 0, 1, 3, or 6 U/kg insulin lispro to evaluate effects of insulin lispro on renal function and electrolyte excretion. Immediately after administration of insulin lispro, the rats were given an oral dose of 25 mL/kg saline solution for hydration. Urine was collected for 5 hours for the determination of volume, pH sodium, potassium, chloride, creatinine, and osmolality. At the end of the urine collection period, blood samples were obtained for the determination of serum sodium, creatinine, and osmolality. Creatinine clearance, osmolal clearance, and fractional excretion of sodium were calculated.

The results of this study demonstrate that a single subcutaneous dose of < 6 U/kg insulin lispro did not result in any serious adverse effects on renal function. However, since changes were observed in one or more parameters at each dose level, a clear no-effect level was not achieved.

Insulin Lispro Protamine Suspension (NPL):

Insulin lispro protamine suspension (NPL) is a formulation in which insulin lispro is co-crystallized with protamine to produce a sustained release preparation analogous to the regular human insulin protamine complex referred to as NPH. The purpose of the animal studies below was to compare the time-action profiles of NPL and NPH. The results suggest that the overall time-action profile of NPL was similar to that of NPH.

A glucose clamp experiment was conducted in dogs to compare the time-action profiles of insulin lispro protamine suspension (NPL) and human insulin (recombinant DNA origin) isophane suspension (NPH). Both insulin preparations used in this study were formulated to contain 100 U/mL. The insulins were administered subcutaneously at a dosage of 0.5 U/kg and the clamp was maintained for 540 minutes. The overall time-action profile of NPL was similar to that of NPH. Insulin lispro concentrations rose slightly faster following NPL administration than the insulin concentrations following NPH administration, but both concentrations decreased at approximately the same rate. The glucose infusion rate remained stable for a longer period of time following NPL but was somewhat lower (20%) at the maximal levels. Otherwise, the glucodynamic effects were similar between the two preparations.

The time-action profile of insulin lispro protamine suspension (NPL) was compared to that of a commercially available insulin protamine isophane suspension (NPH, HUMULIN N) in rabbit blood glucose-lowering tests. Both formulations were administered subcutaneously at 0.2 U/kg to fasted rabbits. The blood glucose profiles of the two laboratory-prepared samples of NPL were similar to NPH. It is concluded that insulin lispro can be modified by co-crystallization with protamine resulting in prolongation of its time-action profile.

Clinical Pharmacology:

Glucose Clamp Studies: Comparison of HUMALOG 100 units/mL to Regular Insulin

A glucose clamp study was performed, in healthy volunteers, in which a 10 U dose of HUMALOG 100 units/mL was compared to HUMULIN R. Doses were given subcutaneously; an additional 10 U dose of intravenous HUMULIN R was given as an absolute reference (Table 4).

HUMALOG 100 units/mL showed statistically higher peak concentrations (C_{max}) which occurred earlier than HUMULIN R (t_{max}). Total absorption was comparable, with serum concentration vs. time area under the curve (AUC) values which were not statistically different.

Table 4. Pharmacokinetics of HUMALOG 100 units/mL Compared with HUMULIN R 100 units/mL in Healthy Volunteers.

Treatment	N	Dose	C_{max} (ng/ml)	t_{max} (min)	AUC (ng•min/mL)
HUMALOG, SC (A)	10	10 U	3.20 ± 1.33	53 ± 30	380 ± 52.2
HUMULIN R, SC (B)	10	10 U	1.79 ± 0.77	101 ± 40	423 ± 71.8
HUMULIN R, IV (C)	10	10 U	58.0 ± 25.1	2 ± 1	601 ± 163
ANOVA results*			<u>A</u> <u>B</u> <u>C</u>	<u>A</u> <u>B</u> <u>C</u>	<u>AB</u> <u>C</u>
<i>p</i> value			< .001	0.001	< .001

*Treatments with statistically comparable values are underlined together.

Glucodynamic data from the same study showed slightly lower maximum glucose infusion rate (R_{max}) values for HUMULIN R when compared to HUMALOG 100 units/mL, although this comparison was not statistically different. However, the time required to achieve this maximum infusion rate (TR_{max}) was significantly earlier for HUMALOG 100 units/mL. The total glucose demand induced by any of the subcutaneous administrations (G_{tot}) were comparable (Table 5).


Table 5. Glucodynamics of HUMALOG 100 units/mL Compared with HUMULIN R 100 units/mL in Healthy Volunteers.

Treatment	R_{max} (mg/min)	TR_{max} (min)	G_{tot} (gm)
HUMALOG, SC (A)	550 ± 203	116 ± 43	85.1 ± 28.2
HUMULIN R, SC (B)	393 ± 180	179 ± 93	81.2 ± 29.9
HUMULIN R, IV (C)	718 ± 247	23 ± 5	50.1 ± 12.9
ANOVA results*	<u>AB</u> <u>C</u>	<u>A</u> <u>B</u> <u>C</u>	<u>AB</u> <u>C</u>
<i>p</i> value	< 0.01	< 0.01	< .001

*Treatments with statistically comparable values are underlined together.

Dose Ranging Studies:

Six differing doses of insulin were administered subcutaneously to each of 18 healthy volunteers. As previously demonstrated the peak insulin level was achieved later and the duration of the glucodynamic effect of HUMULIN R was prolonged as the dose was increased. This study found that the timing of the insulin peak was affected very little by increasing the dose of HUMALOG with only a modest effect in prolonging the duration of the glucose infusion required to balance the increasing doses. Also of interest is the observation of a linear relationship between dose and glucose effect with HUMALOG whereas the relationship was nonlinear for HUMULIN R. This implies that HUMALOG might have a more predictable effect upon glucose levels across the dosage range (Figure 3).

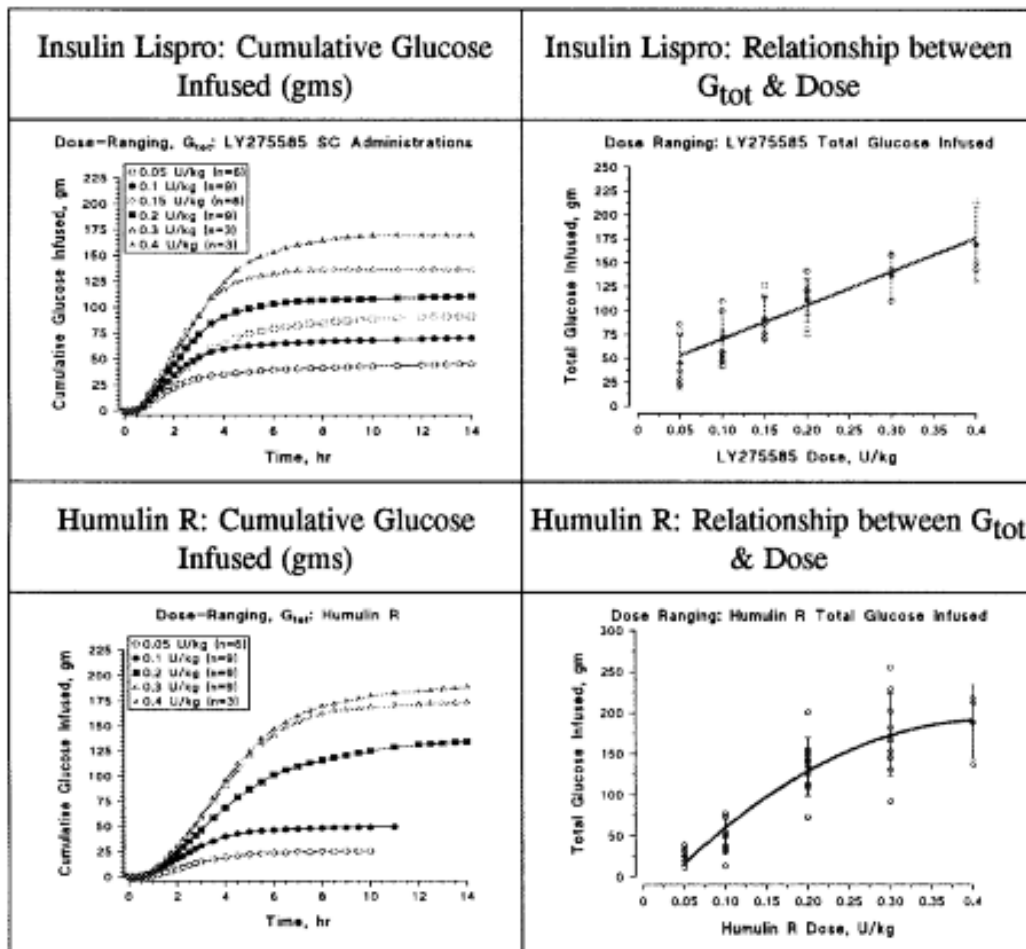

Total Glucose Infused (G_{TOT}) for Insulin Lispro and Humulin R

Figure 3. Dose Ranging Studies in Healthy Volunteers

Comparison of HUMALOG Formulations to Regular Insulin in Patients with type 1 Diabetes

A study was performed comparing the abilities of HUMALOG 100 units/mL and HUMULIN R to control blood glucose after administration of a high calorie meal to patients with type 1 diabetes. Patients were given a low-dose insulin infusion (0.2 mU/kg/min) for basal requirements, then received a dose of either HUMULIN R or HUMALOG 100 units/mL subcutaneously just prior to a meal of pizza, Coke®, and tiramisu (1016 total calories, 57% carbohydrates, 31.6% fat). The dose of subcutaneous regular insulin/ HUMALOG 100 units/mL was selected by the patient based upon previous insulin use, and kept constant between both treatments within any one patient. The mean ± SD subcutaneous HUMULIN R/ HUMALOG dose was 15.4 ± 3.5 U. Whole blood glucose concentrations were measured on a continuous basis after dosing, and blood samples were collected for determination of insulin and HUMALOG concentrations.

The serum drug concentrations confirmed the glucose clamp trial performed in healthy volunteers (Figure 4, Table 6), and shows a more rapid absorption, with HUMALOG 100 units/mL peaking higher and earlier than HUMULIN R. Total absorption was comparable.

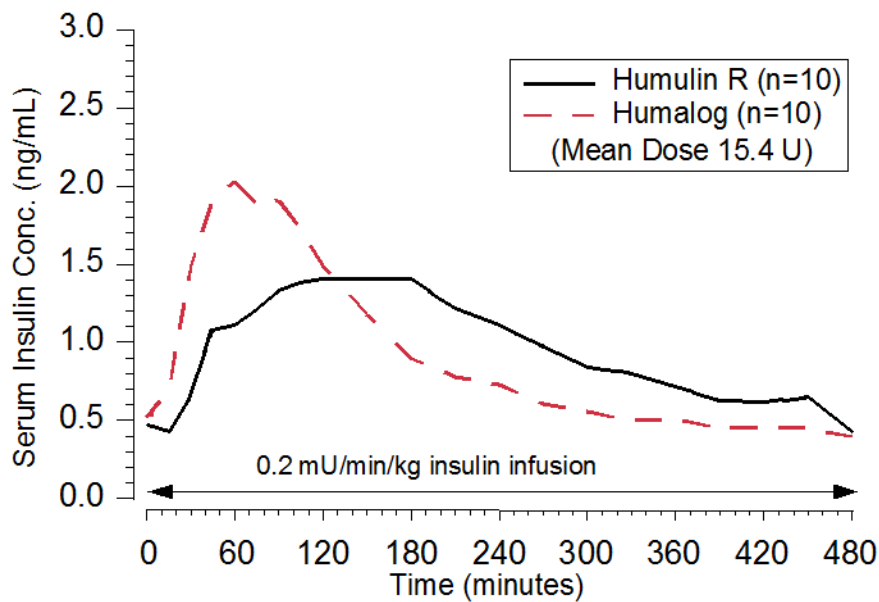


Figure 4. Mean Serum Insulin Concentrations in type 1 Patients Following Injection of HUMULIN R and HUMALOG 100 units/mL (Basal 0.2mU/min/kg insulin infusion).

Table 6. Mean (+/-SD) Pharmacokinetic Parameters, HUMALOG 100 units/mL and HUMULIN R, Adjusted for Insulin Infusion.

Treatment	Dose, U	C _{max} , ng/mL	t _{max} , hr	AUC ₀₋₄ , ng•hr/mL
HUMALOG	15.4 ± 3.5	1.66 ± 0.42	1.13 ± 0.29	3.64 ± 0.88
HUMULIN R	15.4 ± 3.5	1.07 ± 0.30	1.90 ± 0.46	4.05 ± 0.75
<i>p</i> †	--	< 0.001	< 0.001	0.205

Normalized for dose

† Statistical comparisons. P < 0.05 considered statistically significant

Glucose concentrations showed that HUMALOG 100 units/mL controlled the glucose excursions after this meal more completely than did regular insulin (Figure 5). Baseline blood glucose values were attained within 2 hours after meal consumption with HUMALOG 100 units/mL. In comparison, baseline blood glucose was not attained for 4-5 hours after dosing regular insulin. Additionally, a trend was apparent showing a greater potential for regular insulin to induce latent hypoglycemia. However, it should be noted that both insulins were given just prior to the meal, HUMULIN R was not given as recommended in the product label.

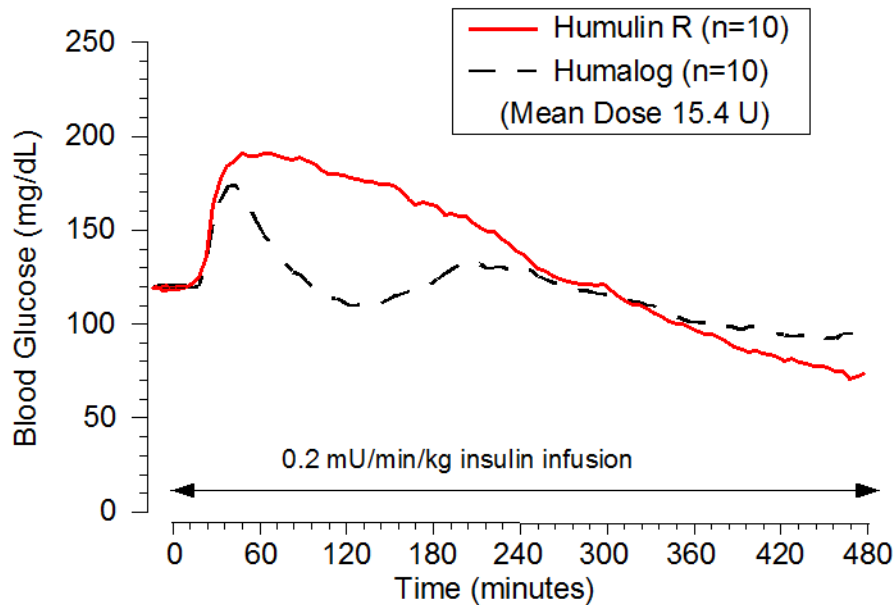


Figure 5. Mean Blood Glucose Concentrations in type 1 Patients Following Injection of HUMULIN R and HUMALOG 100 units/mL Immediately Prior to a Meal.

Comparison of HUMALOG 100 units/mL and HUMALOG 200 units/mL

The pharmacokinetic (PK) and pharmacodynamic (PD) comparability between HUMALOG 200 units/mL and HUMALOG 100 units/mL was evaluated in an 8 hour euglycemic clamp study in 38 healthy subjects following subcutaneous administration of a single 20 unit dose. The results in PK comparison showed the 90% confidence intervals for geometric mean ratio (200 units/mL-to-100 units/mL ratio) of AUC_{inf}, AUC_{last}, and C_{max} were [0.95, 1.04], [0.95, 1.03], and [0.90, 0.97], respectively, all within the [0.8,1.25] bioequivalence boundaries. The median time (t_{max}) to C_{max} values were 60 minutes for HUMALOG 200 units/mL and 45 minutes for HUMALOG 100 units/mL, and the 95% CI for this difference in times (in hours) includes zero [0, 0.25].

The pharmacodynamic responses for HUMALOG 200 units/mL were similar to those for HUMALOG 100 units/mL (Figure 6), with the 90% CI for the ratios of geometric means for the total glucose infused over the duration of the clamp (measure of overall effect) and the maximum glucose infusion rate (measure of maximum effect) contained within the range of 0.80 to 1.25.

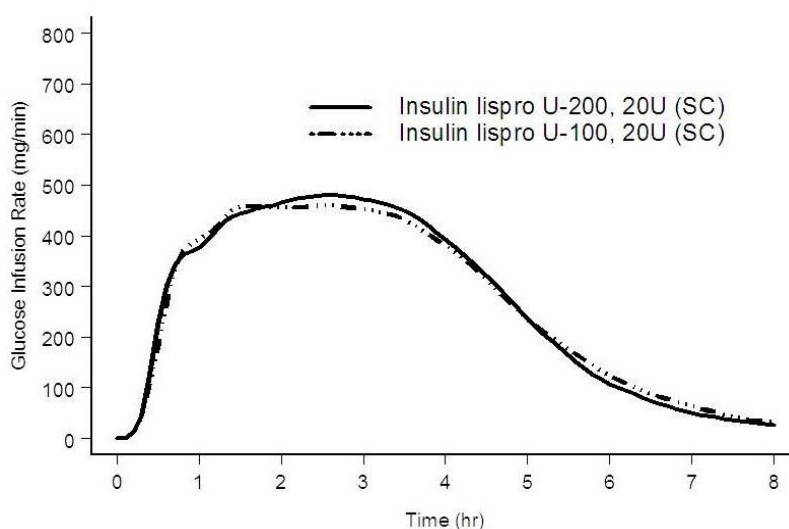


Figure 6. Arithmetic mean glucose infusion rate versus time profiles following the administration of 20 units of HUMALOG 200 units/mL or HUMALOG 100 units/mL


Studies with HUMALOG Mixtures:

Clinical pharmacology studies of mixtures of insulin lispro injection and NPL were designed to demonstrate 1) that the activity profile of NPL is consistent with that of an intermediate-acting insulin (for example, NPH), and 2) that the rapid action of insulin lispro injection is maintained within manufactured insulin lispro injection/NPL mixtures. Four clinical pharmacology studies were completed, three in healthy subjects and one in patients with type 1 diabetes.

One study compared NPL and NPH in a two-way crossover glucose clamp experiment in eight healthy, non-diabetic subjects. A second study confirmed the prolonged duration of activity of NPL by demonstrating its ability to provide overnight blood glucose control in patients with type 1 diabetes when given at bedtime.

Two separate glucose clamp-controlled trials in healthy subjects compared mixtures of insulin lispro injection and NPL with respect to their pharmacokinetic and pharmacodynamic profiles. One of these trials utilized manually-prepared mixtures of insulin lispro injection and NPL while the other employed manufactured fixed mixtures.

NPL provided prolonged insulin activity consistent with that of an intermediate-acting insulin. The rapid onset and peak of activity of insulin lispro injection was maintained within the insulin lispro injection/NPL mixtures. Each mixture studied had a distinct pharmacokinetic and pharmacodynamic profile consistent with the relative proportions of insulin lispro injection and NPL within the mixture (Figure 7).

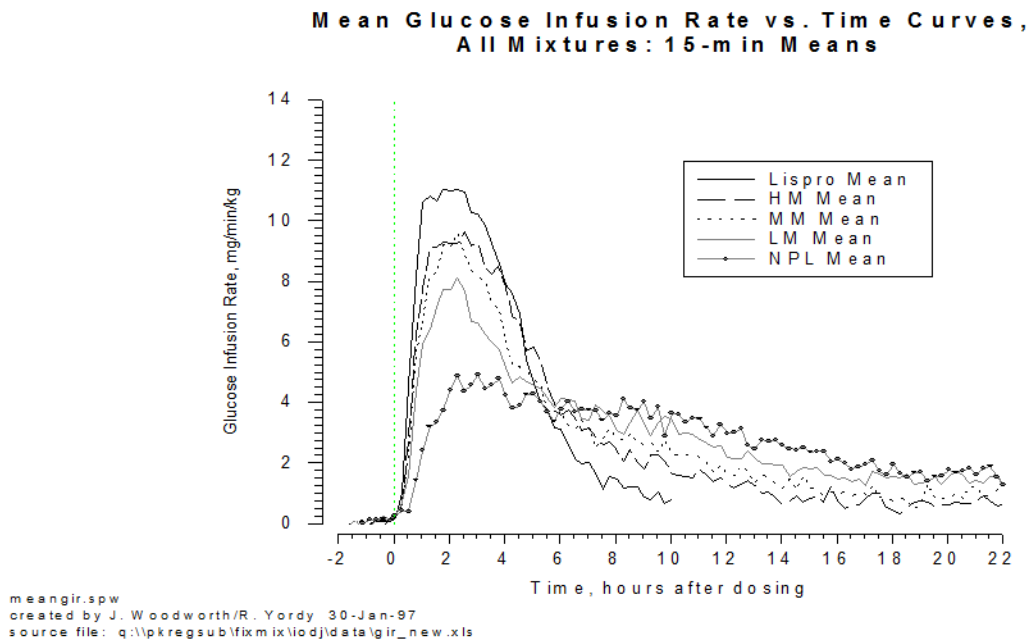

HM - 75% insulin lispro injection, 25% insulin lispro protamine suspension
 MM - 50% insulin lispro injection, 50% insulin lispro protamine suspension
 LM - 25% insulin lispro injection, 75% insulin lispro protamine suspension

Figure 7. Mean Glucose Infusion Rate-Versus-Time Curves

TOXICOLOGY

Acute Toxicity

Table 7. Results of Acute Toxicity Studies with Insulin Lispro

Species, Strain	No./ Sex/ Group; Age	Dose (U/kg)	Route of Administration	Duration of Observations	Parameters Evaluated	Observations
Rat, Fischer 344	5; 8-9 weeks	0, 10	Intravenous	2 weeks	Mortality; clin. obs.; body wt.; pathology	No effects MLD ^a > 10 Units/kg
Rat, Fischer 344	5; 8-9 weeks	0, 10	Subcutaneous	2 weeks	Mortality; clin. obs.; body wt.; pathology	No effects MLD ^a > 10 Units/kg
Rat, Fischer 344	5; 8-9 weeks	0, 10 ^b	Subcutaneous	2 weeks	Mortality; clin. obs.; body wt.; pathology	No effects MLD ^a > 10 Units/kg
Dog, beagle	2; 17-21 months	0, 0.1	Intravenous	2 weeks	Mortality; clin. obs.; body wt.; food consumption; hematology; clin. chemistry	↓ blood glucose MLD ^a > 0.1 Units/kg
Dog, beagle	2; 11-29 months	0, 2	Subcutaneous	2 weeks	Mortality; clin. obs.; body wt.; food consumption; hematology; clin. chemistry	↓ blood glucose MLD ^a > 2 Units/kg

a MLD= median lethal dose

b New formulation with increased *m*-cresol preservative.

Table 8. Results of Acute Toxicity Studies with Insulin Lispro Protamine Suspension (NPL)

Species, Strain	No./ Sex/ Group	Dose (U/kg)	Route of Administration	Duration of Observation	Parameters Evaluated	Observations
Rat, Fischer 344	5	0, 10	Subcutaneous	2 weeks	Mortality; clin. obs.; body wt.; pathology	The median lethal dose of insulin lispro protamine suspension, when administered SC to Fischer 344 rats, was determined to be > 10 units/kg of body weight for males and females. No adverse toxicity was associated

						with insulin lispro protamine suspension.
--	--	--	--	--	--	---

Long-Term Toxicity

Table 9. Results of Subchronic/Chronic Toxicity Studies with Insulin Lispro

Species, Strain	No./Sex/Group; Age	Doses (U/kg/day)	Route of Administration	Duration of Treatment	Parameters Evaluated	Observations
Rat, Fischer 344	10; 4-5 weeks	0, 3	Subcutaneous	1 month	Survival; clin. obs.; ophthalmic exam.; body wt.; food consumption; hematology; clin. chemistry; urinalysis; organ wts.; pathology	No effects.
Dog, beagle	4; 10 months	0, 2	Subcutaneous	1 month	Survival; clin. obs.; ophthalmic & physical exams.; electrocardiograms; body wt.; food consumption; hematology; clin. chemistry; urinalysis; organ wts.; pathology	↓ blood glucose. ↑ heart rate (M, Day 30).
Rat, Fischer 344	15; 7 weeks	0, 5, 20	Subcutaneous	6 months	Survival; clin. obs.; ophthalmic exam.; body wt.; food consumption; hematology; clin. chemistry; urinalysis; organ wts.; pathology	↑ body wt. gain (M & F: 5 & 20 U/kg). ↑ food consumption (F: 20 U/kg). ↑ EFU (M & F: 5 & 20 U/kg). ↓ triglyceride & cholesterol (M & F: 5 & 20 U/kg).
Dog, beagle	4; 7-8 months	0, 1, 2	Subcutaneous	1 year	Survival; clin. obs.; ophthalmic & physical exams.; electrocardiograms; body wt.; food consumption; hematology; clin. chemistry; urinalysis; organ wts.; pathology	↓ blood glucose (M & F: 2 U/kg). ↑ triglyceride & cholesterol. ↑ heart rate & T wave alteration.

Species, Strain	No./Sex/Group; Age	Doses (U/kg/day)	Route of Administration	Duration of Treatment	Parameters Evaluated	Observations
Rat, Fischer 344	30; 7 8 weeks	0, 20, 200	Subcutaneous	1 year	Survival; clin. obs.; ophthalmic exam.; body wt.; food consumption; hematology; clin. chemistry; urinalysis; immunotoxicity; organ wts.; pathology	↑ body wt., body wt. gain; food consumption; EFU (M & F: 200 U/kg) ↑ EFU (F: 20 U/kg) ↑ glucose (M & F: 200 U/kg) ↓ triglycerides (F: 20 & 200 U/kg) ↓ cholesterol (M & F: 20 & 200 U/kg)

Genetic Toxicity

Insulin lispro injection demonstrated no mutagenic potential in five genotoxicity tests. These tests were the induction of reverse mutations in *Salmonella typhimurium* and *Escherichia coli*, induction of unscheduled DNA synthesis in primary cultures of adult rat hepatocytes, induction of mammalian cell mutation in the L5178Y TK[±] mouse lymphoma cell assay, *in vivo* induction of micronuclei in bone marrow of male and female ICR mice, and induction of chromosomal aberrations in Chinese hamster ovary (CHO) cells.

REFERENCES

1. Amiel S, Sherwin R, Simonson D, Taborlane W. Effect of intensive insulin therapy on glycemic thresholds for counterregulatory hormone release. *Diabetes* 1988;37:901-907.
2. Anderson J, Brunelle R, Vignati L. Insulin lispro compared to regular insulin in a crossover study involving 1037 patients with type I diabetes. *Diabetes* 1995;44(Suppl.1):228A.
3. Brems D, Alter L, Beckage M, *et al.* Altering the association properties of insulin by amino acid replacement. *Protein Eng.* 1992;5:527-33.
4. Bastyr III E, Kotsanos J, Vignati L, Cox D. Insulin lispro (LP) reduces hypoglycemia rate in persons with Type II diabetes at high risk for hypoglycemia. *Diabetes* 1994;(Suppl.1):36A.
5. Brunelle R, Anderson J, Vignati L. Decreased rate of hypoglycemia in association with improved metabolic control with insulin lispro. *Diabetologia* 1994;37(Suppl.1):A78.
6. Brunelle R, Symanowski S, Anderson J, Vignati L. Less nocturnal hypoglycemia with insulin lispro in comparison with human regular. *Diabetes* 1995; 44(Suppl. 1):111A.
7. Canadian Diabetes Association 2008 Clinical Practice Guidelines for the Prevention and Management of Diabetes in Canada. *Canadian J. Diabetes* 2008;32 (supp 1):S1-S201.
8. Chantelau E, Heinemann L. Insulin analogs - not faster than U 40 regular human insulin? Letter to editor. *Diabetes Res Clin Pract.* 1993;21:201-202.
9. Cryer P, Binder C, Bolli G, *et al.* Hypoglycemia in IDDM. *Diabetes* 1989;38:1193-1199.
10. Deeb LC, Holcombe J, Brunelle R, *et al.* Insulin lispro lowers postprandial glucose in prepubertal children with diabetes. *Pediatrics* 2001;108(5):1175-1179.
11. Del Sindaco P, Ciofetta M, Lalli C, *et al.* Use of the short-acting insulin analogue lispro in intensive treatment of type 1 diabetes mellitus: importance of appropriate replacement of basal insulin and time-interval injection-meal. *Diabet Med* 1998;15(7):592-600.
12. DiMarchi R, Chance R, Long H, *et al.* Preparation of an insulin with improved pharmacokinetics relative to human insulin through consideration of structural homology with insulin-like growth factor I. *Hormone Res.* 1994;41(suppl 2):93-96.
13. DiMarchi R, Mayer J, Fan L, *et al.* Synthesis of a fast-acting insulin based on structural homology with insulin-like growth factor I. In: Smith JA, Rivier JE, eds. *Peptides, Chemistry and Biology. Proceedings of the Twelfth American Peptide Symposium. Leiden: ESCOM; 1992:26-28.*

14. DiMarchi R. Proinsulin to IGF-I: a family of novel insulin agonists. *Insulin-Dependent Diabetes. Advances in Management, Prevention and Cure.* South Natick MA: IBC USA Conferences Inc; 1992.
15. Ebeling P, Jansson P, Smith U, *et al.* Strategies toward improved control during insulin lispro therapy in IDDM. Importance of basal insulin. *Diabetes Care* 1997;20(8):1287-1289.
16. Gale E. Hypoglycaemia and human insulin. *Lancet* 1989; *ii*:1264-1266.
17. Galloway J, Chance R, Su K. Human insulin and its modifications. In: Reidenberg MM, ed. *The Clinical Pharmacology of Biotechnology Products.* Amsterdam: Elsevier Science Publishers BV (Biomedical Division); 1991:23-34.
18. Galloway J, Chance R. Approaches to insulin analogues. In: Marshall SM, Home PD, eds. *The Diabetes Annual/8.* New York: Elsevier Science; 1994:277-297.
19. Galloway J, Chance R. Insulin agonist therapy: A challenge for the 1990s. *Clin Ther* 1990;12:460-72.
20. Galloway J, Chance R. Insulin analogues. *IDF Bulletin* 1994;39:14-16.
21. Galloway J. New directions in drug development: mixtures, analogues, and modeling. *Diabetes Care* 1993;16 (suppl 3):16-23.
22. Heine R, Bilo H, Fonk T, *et al.* Absorption kinetics and action profiles of mixtures of short-and intermediate-acting insulins. *Diabetologia* 1984;27:558-562.
23. Heinemann L, Starke A, Hohmann A, Berger M. Timing between the subcutaneous administration of insulin and consumption of a carbohydrate rich meal. *Hormone Metabol Res* 1992; 26(Suppl):137-139.
24. Herings R, de Boer A, Stricker B, *et al.* Hypoglycaemia associated with use of inhibitors of angiotensin converting enzyme. *Lancet* 1995;345:1195-1198.
25. Holcombe J, Zalani S, Arora V, *et al.* Lispro in Adolescents Study Group. Comparison of insulin lispro with regular human insulin for the treatment of type 1 diabetes in adolescents. *Clin Ther* 2002;24(4):629-38.
26. Howey D, Bowsher R, Brunelle R, *et al.* [Lys(B28), Pro(B29)]-Human insulin: a rapidly absorbed analogue of human insulin. *Diabetes* 1994;43:396-402.
27. Jacobs M, Heine R. Insulin analogues: new horizons or false dawns? In: Barnett AH, ed. *Diabetes. Reviews 2/4.* London: Macmillan Magazines; 1993:2-4.

28. Jansson P, Ebeling P, Smith U, *et al.* Improved glycemic control can be better maintained with insulin lispro than with human regular insulin. *Diab Nutr Metab* 1998;11:194-99.
29. Joseph S, Korzon-Burakowska A, *et al.* The Action Profile of Lispro is Not Blunted by Mixing in the Syringe With NPH Insulin. *Diabetes Care* 1998;21:2098-2102.
30. Kurtz W, Pravenec M. Antidiabetic mechanisms of angiotensin-converting-enzyme inhibitors and angiotensin II receptor antagonists: beyond: the renin-angiotensin system. *J Hypertension* 2004; 22(12):2253-2261.
31. Lalli C, Ciofetta M, Del Sindaco P, *et al.* Long-term intensive treatment of type 1 diabetes with the short-acting insulin analog lispro in variable combination with NPH insulin at mealtime. *Diabetes Care* 1999;22(3):468-77.
32. Pedersen-Bjergaard U, Agerholm-Larsen B, Pramming S, *et al.* Activity of angiotensin-converting enzyme and risk of severe hypoglycaemia in type 1 diabetes mellitus. *Lancet* 2001;357:1248-1253.
33. Scherthaner G, Wein W, Sandholzer K, *et al.* Postprandial insulin lispro. A new therapeutic option for type 1 diabetic patients. *Diabetes Care* 1998;21(4):570-3.
34. Slieker L, Brooke G, Chance R, *et al.* Insulin and IGF-I analogs: Novel approaches to improved insulin pharmacokinetics. In: LeRoith D, Raizada MK, eds. *Current Directions in Insulin-Like Growth Factor Research*. New York: Plenum Press;1994:25-32.
35. Stiller R, Gudat U, Pfützner A, *et al.* Postprandial treatment with insulin lispro. *Diabetes & Metabolism* 1997;23:232-233.
36. Teuscher A, Berger W. Hypoglycaemia unawareness in diabetics transferred from beef/porcine insulin to human insulin. *Lancet* 1987.
37. The Diabetes Control and Complications Trial Research Group. The effect of intensive treatment of diabetes on the development and progression of long-term complications in insulin-dependent diabetes mellitus. *N Engl J Med* 1993;329:977-986.
38. Torlone E, Fanelli C, Rambotti A, *et al.* Pharmacokinetics, pharmacodynamics and glucose counterregulation following subcutaneous injection of the monomeric insulin analogue [Lys(B28),Pro(B29)] in IDDM. *Diabetologia* 1994;37:713-720.
39. Van Bon AC, Brouwer TB, von Basum G, *et al.* Insulin glulisine compared to insulin aspart and to insulin lispro administered by continuous subcutaneous insulin infusion in patients with type 1 diabetes: a randomized controlled trial. *Diabetes Technol Ther* 2011;13(6):607-614.

40. Vignati L, Brunelle R. Treatment of 722 patients with type 2 diabetes with insulin lispro: A 6 month crossover study. *Diabetes* 1994;44(Suppl 1): 229A.

PART III: CONSUMER INFORMATION

HUMALOG® VIALS

(insulin lispro injection)

Solution for Injection, 100 units/mL, Lilly Standard

This leaflet is part III of a three-part "Product Monograph" published when HUMALOG® was approved for sale in Canada and is designed specifically for Consumers. This leaflet is a summary and will not tell you everything about HUMALOG®. Contact your doctor or pharmacist if you have any questions about the drug.

ABOUT THIS MEDICATION

What the medication is used for:

Insulin is a hormone produced by the pancreas, a large gland that lies near the stomach. This hormone is necessary for the body's correct use of food, especially sugar. Diabetes occurs when the pancreas does not make enough insulin to meet your body's needs.

To control your diabetes, your doctor has prescribed injections of insulin to keep your blood glucose at a near-normal level.

What it does:

Insulin lispro is a recombinant DNA sourced human insulin analogue. HUMALOG consists of zinc-insulin lispro crystals dissolved in a clear fluid. HUMALOG is used to control high blood sugar (glucose) in people with diabetes. HUMALOG takes effect more rapidly and has a shorter duration of activity as compared to regular insulin.

The rapid onset of activity requires HUMALOG to be given within 15 minutes before a meal. When necessary, HUMALOG may be given shortly after a meal instead (within 20 minutes of the start of the meal). The time course of action of any insulin may vary to some extent in different individuals or at different times in the same individual. As with all insulin preparations, the duration of action of HUMALOG is dependent on dose, site of injection, blood supply, temperature, and physical activity.

Proper control is important. Uncontrolled diabetes (hyperglycemia) over a long period of time can result in a number of serious problems such as blindness, kidney failure, poor circulation/heart attacks, strokes and/or nerve damage. These problems can be prevented or reduced by good diabetes management. This will require close and constant cooperation with your diabetes healthcare team including: yourself, your doctor and your diabetes educators (nurses, dietitians, social workers, pharmacists and other healthcare professionals). Thus, you can lead an active, healthy and productive life by eating a balanced daily diet, exercising regularly, and taking your insulin injections as prescribed.

You have been instructed to test your blood and/or your urine regularly for glucose. If your blood tests consistently show above- or below-normal glucose levels or your urine tests

consistently show the presence of glucose, your diabetes is not properly controlled and you must let your doctor know.

When it should not be used:

- When your blood sugar is too low (hypoglycemia). After treating your low blood sugar, follow your healthcare provider's instructions on the use of HUMALOG.
- If you are allergic to anything in HUMALOG. A complete list of ingredients in HUMALOG is provided below.

What the medicinal ingredient is:

HUMALOG contains 100 units/mL of Human Insulin Analogue.

HUMALOG contains insulin lispro injection.

What the non-medicinal ingredients are:

HUMALOG contains glycerol, dibasic sodium phosphate, m-cresol, zinc (as ion) and water for injection. Hydrochloric acid or sodium hydroxide may be added to adjust pH.

What dosage forms it comes in:

HUMALOG is a sterile solution containing insulin lispro injection. It is available in:

- Vial, 10 mL
- Vial, 3 mL

HUMALOG is also available in:

- Cartridge, 3 mL
- KwikPen, 3 mL prefilled pen
- Junior KwikPen, 3 mL prefilled pen

Other HUMALOG products include:

- HUMALOG 200 units/mL KwikPen (insulin lispro injection)
- HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension)
- HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension)

DO NOT USE ANY OTHER INSULIN EXCEPT ON YOUR DOCTOR'S ADVICE AND DIRECTION.

Always keep an extra supply of HUMALOG as well as a spare syringe and needle or injection device on hand. Always wear identification to indicate that you have diabetes so that appropriate treatment can be given if complications occur away from home.

When you receive your insulin from the pharmacy, always check to see that:

1. The name HUMALOG appears on the carton and bottle (vial) label.
2. The carton and bottle (vial) label is correct for your type of insulin.
3. The insulin strength is U-100.

- The expiration date on the package will allow you to use the insulin before that date.

WARNINGS AND PRECAUTIONS

Serious Warnings and Precautions

- Hypoglycemia or low blood sugar is the most common adverse effect experienced by insulin users. Blood glucose monitoring is recommended for all patients with diabetes. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma or even death. Information on how to recognize these symptoms is provided below.
- This Lilly human insulin analogue differs from other insulins because it has a unique structure, a very quick onset of action and a short duration of activity. HUMALOG should be given within 15 minutes before a meal or when necessary shortly after a meal instead (within 20 minutes of the start of the meal). The short duration of action of HUMALOG means that if you have Type 1 diabetes you also need to use a longer-acting insulin to give the best glucose control (except when using an insulin infusion pump).
- HUMALOG should not be used if it is not water-clear and colourless or if it has formed a deposit of solid particles on the wall of the vial.
- Any change of insulin regimen should be made cautiously and only under medical supervision. Changes in purity, strength, brand (manufacturer), type (regular, NPH, etc), species (beef, pork, beef-pork, human), and/or method of manufacture (recombinant DNA versus animal-source insulin) may result in the need for a change in dosage.
- Mixing of HUMALOG with either animal insulins or insulin preparations produced by other manufacturers is not recommended.
- Patients taking HUMALOG may require a change in dosage from that used with other insulins. If an adjustment is needed, it may occur with the first dose or over a period of several weeks.
- Insulin infusion pump: when used in an insulin infusion pump, HUMALOG should not be diluted or mixed with any other insulin. Carefully read and follow the insulin infusion pump manufacturer's instructions and this insert before using HUMALOG.

BEFORE you use HUMALOG talk to your doctor or pharmacist if:

- You have trouble with your kidneys or liver, your doctor may decide to alter your insulin dose.
- You drink alcohol (including wine and beer): watch for signs of hypoglycemia and never drink alcohol on an empty stomach.
- You exercise more than usual or if you want to change your usual diet. Exercise may lower your body's need for insulin during and for some time after the activity. Exercise may

also speed up the effect of an insulin dose, especially if the exercise involves the area of injection site.

- You are ill. Illness, especially with nausea and vomiting, may cause your insulin requirements to change. Even if you are not eating, you will still require insulin. You and your doctor should establish a sick day plan for you to use in case of illness. When you are sick, test your blood/urine frequently.
- You are travelling across more than 2 time zones. You should consult your doctor concerning adjustments in your insulin schedule.
- You are pregnant. HUMALOG can be used in pregnancy if clinically indicated. Data on a large number of exposed pregnancies do not indicate any adverse effect of HUMALOG on pregnancy or on the health of the foetus/newborn. Good control of diabetes is especially important for you and your unborn baby. Pregnancy may make managing your diabetes more difficult. If you are planning to have a baby, are pregnant, or are nursing a baby, consult your doctor.
- When you use other medicines. Many medicines affect the way glucose works in your body and this may influence your insulin dose. Listed below are the most common medicines, which may affect your insulin treatment. Talk to your doctor or pharmacist if you take, or change any other medicines, even those not prescribed.

INTERACTIONS WITH THIS MEDICATION

Insulin requirements may be increased if you are taking other drugs with hyperglycemic activity, such as oral contraceptives (for example, birth control pills, injections and patches), corticosteroids, or thyroid replacement therapy. Insulin requirements may be decreased in the presence of agents such as oral antidiabetic agents, salicylates (aspirin), sulfa antibiotics, certain antidepressants (monoamine oxidase inhibitors), beta-blockers, alcohol, ACE-inhibitors and angiotensin II receptor blockers. Always discuss any medications you are taking with your doctor.

The use of thiazolidinediones (such as rosiglitazone and pioglitazone), alone or in combination with other antidiabetic agents (including insulin), has been associated with heart failure and swelling of the lower extremities. Please contact your physician immediately if you develop symptoms of shortness of breath, fatigue, exercise intolerance, or swelling of the lower extremities while you are on these agents.

PROPER USE OF THIS MEDICATION

HUMALOG is a sterile solution. HUMALOGs should be given by subcutaneous injection, or by continuous subcutaneous insulin infusion pump. The concentration of HUMALOG in 3 mL vials or 10 mL vials is 100 units/mL (U-100).

When used as a meal-time insulin, HUMALOGs should be given within 15 minutes before a meal, or when necessary shortly after a meal instead (within 20 minutes of the start of the meal).

HUMALOG is a clear and colourless liquid with a water-like appearance and consistency. Do not use if it appears cloudy, thickened, or slightly coloured or if solid particles are visible. Always check the appearance of your vial of HUMALOG before using, and if you note anything unusual in its appearance or notice your insulin requirements changing markedly, consult your doctor.

Injection Procedure

Correct Syringe:

Doses of insulin are measured in units. HUMALOG is available in 100 units/mL (U-100). It is important that you understand the markings on your syringe, because the volume of HUMALOG you inject depends on the strength, that is, the number of units/mL. For this reason, you should always use a syringe marked for U-100 insulin preparations. Failure to use the proper syringe can lead to a mistake in dosage, causing serious problems for you, such as a blood glucose level that is too low or too high.

Syringe Use:

To help avoid contamination and possible infection, follow these instructions exactly.

Disposable plastic syringes and needles should be used only once and then discarded in a closable, puncture-resistant sharps container (like a biohazard container) or as directed by your healthcare professional. **NEEDLES AND SYRINGES MUST NOT BE SHARED**, as this may risk transmission of infectious agents.

Reusable glass syringes and needles must be sterilized before each injection. **Follow the package directions supplied with your syringe.**

Preparing the Dose:

1. Wash your hands.
2. Inspect the HUMALOG in the vial. It should look clear and colourless. Do not use HUMALOG if it appears cloudy, thickened, or slightly coloured or if solid particles are visible.
3. Flip off the plastic protective cap but do not remove the stopper if using a new vial.
4. Wipe the top of the vial with an alcohol swab.
5. If you are mixing insulins, refer to the instructions for mixing below.
6. Remove the cover from the needle. Draw air into the syringe equal to your HUMALOG dose. Put the needle through the rubber top of the HUMALOG vial and inject the air into the vial.
7. Turn the vial and syringe upside down. Hold the vial and syringe firmly in one hand.
8. Making sure the tip of the needle is in the HUMALOG, withdraw the correct dose into the syringe.

9. Before removing the needle from the vial, check your syringe for air bubbles, which reduce the amount of HUMALOG. If bubbles are present, hold the syringe straight up and tap its side until the bubbles float to the top. Push them out with the plunger and withdraw the correct dose.
10. Remove the needle from the vial and lay the syringe down so that the needle does not touch anything.

Mixing HUMALOG With Long-Acting Insulin Formulations

MIXING HUMALOG WITH EITHER ANIMAL INSULINS OR INSULIN PREPARATIONS PRODUCED BY OTHER MANUFACTURERS IS NOT RECOMMENDED.

1. HUMALOG should be mixed with long-acting insulins (HUMULIN N) only on the advice of your doctor.
2. Draw air into your syringe equal to the amount of longer-acting HUMULIN insulin you are taking. Insert the needle into the long-acting insulin vial and inject the air, taking care not to come in contact with the insulin in the vial. Withdraw the needle.
3. Now inject air into your HUMALOG vial in the same manner, but do not withdraw the needle.
4. Turn the vial and syringe upside down.
5. Making sure the tip of the needle is in the HUMALOG, withdraw the correct dose of HUMALOG into the syringe.
6. Before removing the needle from the vial of HUMALOG, check your syringe for air bubbles, which reduce the amount of HUMALOG in it. If bubbles are present, hold the syringe straight up and tap its side until the bubbles float to the top. Push them out with the plunger and withdraw the correct dose. Gently roll or shake the long-acting HUMULIN vial until the insulin is mixed.
7. Remove the needle from the vial of HUMALOG and insert it into the vial of the long-acting HUMULIN insulin. Turn the vial and syringe upside down. Making sure the tip of the needle is in the insulin, withdraw your dose of long-acting HUMULIN insulin.
8. Remove the needle and lay the syringe down so that the needle does not touch anything.

Follow your doctor's instructions on mixing your insulin just before giving your injection. HUMALOG should be injected immediately after mixing. It is important to be consistent in your method.

Syringes from different manufacturers may vary in the amount of space between the bottom line and the needle. Because of this, do not change the sequence of mixing, or the model and brand of syringe or needle that the doctor has prescribed.

Injection:

Prepare the injection site as directed by your healthcare professional. To avoid tissue damage (skin thinning, skin

thickening, or skin lumps), always change the site for each injection by at least 1.5 cm (0.5 inches) from the previous site, rotating sites on the body so that the same site is not used more than approximately once a month. Do not inject into pits (depressions), thickened skin or lumps.

Insert the needle as instructed by your doctor. Push the plunger in as far as it will go. Pull the needle out and apply gentle pressure over the injection site for several seconds. Do not rub the area.

Use of HUMALOG in an Insulin Infusion Pump:

1. Health Canada approved insulin infusion pumps may be used to infuse HUMALOG U-100. Read and follow the instructions that accompany the infusion pump.
2. Be sure to use the correct reservoir and catheter for the pump.
3. Change the HUMALOG in the reservoir at least every 14 days. Change the infusion set as recommended in pump manufacturers' instructions (typically every 3 days is recommended) or as directed by your healthcare professional. Use aseptic technique when inserting the infusion set.
4. In the event of a hypoglycemic episode, the infusion should be stopped until the episode is resolved. If repeated or severe low blood glucose levels occur, notify your health care professional and consider the need to reduce or temporarily stop your insulin infusion.
5. A pump malfunction or obstruction of the infusion set can result in a rapid rise in glucose levels. If an interruption to insulin flow is suspected, follow the instructions in the product literature and if appropriate, notify your health care professional.
6. When used with an insulin infusion pump, HUMALOG should not be mixed with any other insulin.

Usual dose

Your doctor has told you which insulin to use, how much, and when and how often to inject it. Because each patient's case of diabetes is different, this schedule has been individualized for you.

Your usual HUMALOG dose may be affected by changes in your food, activity, or work schedule. Carefully follow your doctor's instructions to allow for these changes. Other things that may affect your HUMALOG dose are illness, pregnancy, medication, exercise and travel.

Overdose

Hypoglycemia (too little glucose in the blood) is one of the most frequent adverse events experienced by insulin users. It can be brought about by:

1. Missing or delaying meals
2. Taking too much insulin
3. Exercising or working more than usual
4. An infection or illness (especially with diarrhea or vomiting)
5. A change in the body's need for insulin

6. Diseases of the adrenal, pituitary, or thyroid gland, or progression of kidney or liver disease
7. Interactions with other drugs that lower blood glucose, such as oral hypoglycemics, salicylates, sulfa antibiotics, and certain antidepressants
8. Consumption of alcoholic beverages

Dietary Implications:

If a usual meal cannot be obtained at the appropriate time, then to avoid hypoglycemia, you should take the amount of carbohydrate prescribed for this meal in the form of orange juice, syrup, candy, or bread and milk, without changing your insulin dosage. If it becomes necessary to omit a meal on account of nausea and vomiting, you should test your blood sugar level and notify your doctor.

Mild to moderate hypoglycemia may be treated by eating foods or drinks that contain sugar. Patients should always carry a quick source of sugar, such as candy mints or glucose tablets. More severe hypoglycemia may require the assistance of another person. Patients who are unable to take sugar orally or who are unconscious should be treated with intravenous administration of glucose at a medical facility or should be given an injection of glucagon (either intramuscular or subcutaneous). The patient should be given oral carbohydrates as soon as consciousness is recovered.

In case of drug overdose, contact a healthcare practitioner, hospital emergency department or regional Poison Control Centre immediately, even if there are no symptoms.

SIDE EFFECTS AND WHAT TO DO ABOUT THEM

Hypoglycemia:

One of the most frequent adverse events experienced by insulin users is hypoglycemia (see PROPER USE OF THIS MEDICATION).

Diabetic Acidosis and Coma:

Diabetic acidosis may develop if your body has too little insulin (this is the opposite of insulin reaction, which is the result of too much insulin in the blood). Diabetic acidosis may be brought on if you omit your insulin or take less than the doctor has prescribed, eat significantly more than your diet calls for, or develop a fever or infection. With acidosis, urine tests show a large amount of sugar and acetone.

The first symptoms of diabetic acidosis usually come on gradually, over a period of hours or days, and include a drowsy feeling, flushed face, thirst, and loss of appetite. Heavy breathing and a rapid pulse are more severe symptoms.

If uncorrected, loss of consciousness, coma, or death can result. Therefore, it is important that you obtain medical assistance immediately.

Lipoatrophy, Lipohypertrophy, or Localized Cutaneous Amyloidosis:

Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the skin), lipohypertrophy (enlargement or thickening of tissue), or localized cutaneous amyloidosis (skin lumps). If you notice any of these conditions, consult your doctor. A change in your injection technique may help alleviate the problem.

Allergy to Insulin:

Patients occasionally experience redness, swelling, and itching at the site of injection of insulin. This condition, called local allergy, usually clears up in a few days to a few weeks. If you have local reactions, contact your doctor, who may recommend a change in the type or species of insulin.

Less common, but potentially more serious, is generalized allergy to insulin, which may cause rash over the whole body, shortness of breath, wheezing, reduction in blood pressure, fast pulse, or sweating. Severe cases of generalized allergy may be life threatening. If you think you are having a generalized allergic reaction to insulin, notify a doctor immediately. Your doctor may recommend skin testing, that is, injecting small doses of other insulins into the skin, in order to select the best insulin for you to use. Patients who have had severe generalized allergic reactions to insulin should be skin tested with each new preparation to be used before treatment with that preparation is started.

This is not a complete list of side effects. For any unexpected effects while taking HUMALOG, contact your doctor or pharmacist.

HOW TO STORE IT

Prior to first use, HUMALOG insulin vials should be stored in a refrigerator between 2° and 8°C. Do not freeze. Do not expose to excessive heat or sunlight. The vial of HUMALOG that you are currently using can be kept unrefrigerated, for up to 28 days, as long as it is kept as cool as possible (below 30°C) and away from direct heat and light. Vials in use, or not refrigerated, should be discarded after 28 days even if they still contain HUMALOG. Do not use HUMALOG if it has been frozen.

DO NOT USE A VIAL OF HUMALOG AFTER THE EXPIRATION DATE STAMPED ON THE LABEL.

REPORTING SUSPECTED SIDE EFFECTS

You can report any suspected adverse reactions associated with the use of health products to the Canada Vigilance Program by one of the following 3 ways:

- Report online at www.healthcanada.gc.ca/medeffect
- Call toll-free at 1-866-234-2345
- Complete a Canada Vigilance Reporting Form and:
 - Fax toll-free to 1-866-678-6789, or
 - Mail to:
 - Canada Vigilance Program
 - Health Canada
 - Postal Locator 0701D
 - Ottawa, Ontario
 - K1A 0K9

Postage paid labels, Canada Vigilance Reporting Form and the adverse reaction reporting guidelines are available on the MedEffect™ Canada Web site at www.healthcanada.gc.ca/medeffect

NOTE: Should you require information related to the management of side effects, contact your health professional. The Canada Vigilance Program does not provide medical advice.

MORE INFORMATION

For more information, please contact your healthcare professionals or pharmacist first, or Eli Lilly Canada Inc. at:

1-888-545-5972 or visit the website at www.lilly.ca.

The information in this document is current as of the last revision date shown below. For the most current information please visit our website or contact us directly.

This leaflet was prepared by Eli Lilly Canada Inc.

HUMALOG, MIX25, MIX50 and KwikPen are registered trademarks owned by Eli Lilly and Company, its subsidiaries or affiliates.

You may need to read this package insert again. Please do not throw it away until you have finished your medicine.

Last revised: Month DD, 2021

LOGVL-0003-CA-PMI-2021MMDD

PART III: CONSUMER INFORMATION

HUMALOG® CARTRIDGES

(insulin lispro injection)

Solution for Injection, 100 units/mL, Lilly Standard

HUMALOG® KWIKPEN®

(insulin lispro injection)

Solution for Injection, 100 units/mL, Lilly Standard

HUMALOG® JUNIOR KWIKPEN®

(insulin lispro injection)

Solution for Injection, 100 units/mL, Lilly Standard

This leaflet is part III of a three-part "Product Monograph" published when HUMALOG® was approved for sale in Canada and is designed specifically for Consumers. This leaflet is a summary and will not tell you everything about HUMALOG®. Contact your doctor or pharmacist if you have any questions about the drug.

ABOUT THIS MEDICATION

What the medication is used for:

Insulin is a hormone produced by the pancreas, a large gland that lies near the stomach. This hormone is necessary for the body's correct use of food, especially sugar. Diabetes occurs when the pancreas does not make enough insulin to meet your body's needs.

To control your diabetes, your doctor has prescribed injections of insulin to keep your blood glucose at a near-normal level.

What it does:

Insulin lispro is a recombinant DNA sourced human insulin analogue. HUMALOG consists of zinc-insulin lispro crystals dissolved in a clear fluid. HUMALOG is used to control high blood sugar (glucose) in people with diabetes. HUMALOG takes effect more rapidly and has a shorter duration of activity as compared to regular insulin.

The rapid onset of activity requires HUMALOG to be given within 15 minutes before a meal. When necessary, HUMALOG may be given shortly after a meal instead (within 20 minutes of the start of the meal). The time course of action of any insulin may vary to some extent in different individuals or at different times in the same individual. As with all insulin preparations, the duration of action of HUMALOG is dependent on dose, site of injection, blood supply, temperature, and physical activity.

Proper control is important. Uncontrolled diabetes (hyperglycemia) over a long period of time can result in a number of serious problems such as blindness, kidney failure, poor circulation/heart attacks, strokes and/or nerve damage. These problems can be prevented or reduced by good diabetes management. This will require close and constant cooperation with your diabetes healthcare team including: yourself, your doctor and your diabetes educators (nurses, dietitians, social

workers, pharmacists and other healthcare professionals). Thus, you can lead an active, healthy and productive life by eating a balanced daily diet, exercising regularly, and taking your insulin injections as prescribed.

You have been instructed to test your blood and/or your urine regularly for glucose. If your blood tests consistently show above- or below-normal glucose levels or your urine tests consistently show the presence of glucose, your diabetes is not properly controlled and you must let your doctor know.

When it should not be used:

- When your blood sugar is too low (hypoglycemia). After treating your low blood sugar, follow your healthcare provider's instructions on the use of HUMALOG.
- If you are allergic to anything in HUMALOG. A complete list of ingredients in HUMALOG is provided below.

What the medicinal ingredient is:

HUMALOG contains 100 units/mL of Human Insulin Analogue.

HUMALOG contains insulin lispro injection.

What the non-medicinal ingredients are:

HUMALOG contains glycerol, dibasic sodium phosphate, m-cresol, zinc (as ion) and water for injection. Hydrochloric acid or sodium hydroxide may be added to adjust pH.

What dosage forms it comes in:

HUMALOG is a sterile solution containing insulin lispro injection. It is available in:

- Cartridge, 3 mL
- KwikPen, 3 mL prefilled pen
- Junior KwikPen, 3 mL prefilled pen

HUMALOG is also available in:

- Vial, 10 mL
- Vial, 3 mL

Other HUMALOG products include:

- HUMALOG 200 units/mL KwikPen (insulin lispro injection)
- HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension)
- HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension)

HUMALOG prefilled pens and cartridges are available in boxes of 5. HUMALOG cartridges are designed for use with Lilly injector systems. The cartridge or prefilled pen containing HUMALOG is not designed to allow any other insulin to be mixed in the cartridge or for the cartridge or prefilled pen to be reused.

For guidance on the use of the Pen (prefilled, disposable insulin injector), please refer to the separate Instructions for Use enclosed within the packaging.

DO NOT USE ANY OTHER INSULIN EXCEPT ON YOUR DOCTOR'S ADVICE AND DIRECTION.

Always keep an extra supply of HUMALOG i.e. a spare pen and cartridge or prefilled pen on hand. Always wear identification to indicate that you have diabetes so that appropriate treatment can be given if complications occur away from home.

When you receive your insulin from the pharmacy, always check to see that:

1. The name HUMALOG appears on the carton and cartridge or prefilled pen label.
2. The carton and cartridge or prefilled pen label is correct for your type of insulin.
3. The insulin strength is U-100.
4. The expiration date on the package will allow you to use the insulin before that date.

WARNINGS AND PRECAUTIONS

Serious Warnings and Precautions

- Hypoglycemia or low blood sugar is the most common adverse effect experienced by insulin users. Blood glucose monitoring is recommended for all patients with diabetes. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma or even death. Information on how to recognize these symptoms is provided below.
- This Lilly human insulin analogue differs from other insulins because it has a unique structure, a very quick onset of action and a short duration of activity. HUMALOG should be given within 15 minutes before a meal or when necessary shortly after a meal instead (within 20 minutes of the start of the meal). The short duration of action of HUMALOG means that if you have Type 1 diabetes you also need to use a longer-acting insulin to give the best glucose control (except when using an insulin infusion pump).
- HUMALOG should not be used if it is not water-clear and colourless or if it has formed a deposit of solid particles on the wall of the cartridge.
- Any change of insulin regimen should be made cautiously and only under medical supervision. Changes in purity, strength, brand (manufacturer), type (regular, NPH, etc), species (beef, pork, beef-pork, human), and/or method of manufacture (recombinant DNA versus animal-source insulin) may result in the need for a change in dosage.
- Mixing of HUMALOG with either animal insulins or insulin preparations produced by other manufacturers is not recommended.
- Patients taking HUMALOG may require a change in dosage from that used with other insulins. If an

adjustment is needed, it may occur with the first dose or over a period of several weeks.

- **Insulin infusion pump:** when used in an insulin infusion pump, HUMALOG should not be diluted or mixed with any other insulin. Carefully read and follow the insulin infusion pump manufacturer's instructions and this insert before using HUMALOG.

BEFORE you use HUMALOG talk to your doctor or pharmacist if:

- You have trouble with your kidneys or liver, your doctor may decide to alter your insulin dose.
- You drink alcohol (including wine and beer): watch for signs of hypoglycemia and never drink alcohol on an empty stomach.
- You exercise more than usual or if you want to change your usual diet. Exercise may lower your body's need for insulin during and for some time after the activity. Exercise may also speed up the effect of an insulin dose, especially if the exercise involves the area of injection site.
- You are ill. Illness, especially with nausea and vomiting, may cause your insulin requirements to change. Even if you are not eating, you will still require insulin. You and your doctor should establish a sick day plan for you to use in case of illness. When you are sick, test your blood/urine frequently.
- You are travelling across more than 2 time zones. You should consult your doctor concerning adjustments in your insulin schedule.
- You are pregnant. HUMALOG can be used in pregnancy if clinically indicated. Data on a large number of exposed pregnancies do not indicate any adverse effect of HUMALOG on pregnancy or on the health of the foetus/newborn. Good control of diabetes is especially important for you and your unborn baby. Pregnancy may make managing your diabetes more difficult. If you are planning to have a baby, are pregnant, or are nursing a baby, consult your doctor.
- When you use other medicines. Many medicines affect the way glucose works in your body and this may influence your insulin dose. Listed below are the most common medicines, which may affect your insulin treatment. Talk to your doctor or pharmacist if you take, or change any other medicines, even those not prescribed.

INTERACTIONS WITH THIS MEDICATION

Insulin requirements may be increased if you are taking other drugs with hyperglycemic activity, such as oral contraceptives (for example, birth control pills, injections and patches), corticosteroids, or thyroid replacement therapy. Insulin requirements may be decreased in the presence of agents such as oral antidiabetic agents, salicylates (aspirin), sulfa antibiotics, certain antidepressants (monoamine oxidase inhibitors), beta-blockers, alcohol,

ACE-inhibitors and angiotensin II receptor blockers. Always discuss any medications you are taking with your doctor.

The use of thiazolidinediones (such as rosiglitazone and pioglitazone), alone or in combination with other antidiabetic agents (including insulin), has been associated with heart failure and swelling of the lower extremities. Please contact your physician immediately if you develop symptoms of shortness of breath, fatigue, exercise intolerance, or swelling of the lower extremities while you are on these agents.

PROPER USE OF THIS MEDICATION

HUMALOG is a sterile solution. HUMALOG should be given by subcutaneous injection, or by continuous subcutaneous insulin infusion pump. The concentration of HUMALOG in 3 mL cartridges or prefilled pens is 100 units/mL (U-100).

When used as a meal-time insulin, HUMALOG should be given within 15 minutes before a meal, or when necessary shortly after a meal instead (within 20 minutes of the start of the meal).

HUMALOG is a clear and colourless liquid with a water-like appearance and consistency. Do not use if it appears cloudy, thickened, or slightly coloured or if solid particles are visible. Always check the appearance of your cartridge or prefilled pen of HUMALOG before using, and if you note anything unusual in its appearance or notice your insulin requirements changing markedly, consult your doctor.

Injection Procedure

Preparing a Cartridge of HUMALOG for Insertion in a Pen:

1. Wash your hands.
2. Before inserting the HUMALOG cartridge into the pen, inspect it to make sure the contents look clear and colourless. Do not use the HUMALOG cartridge if it appears cloudy, thickened, or slightly coloured or if solid particles are visible or if the cartridge is cracked or broken.
3. Follow the pen manufacturer's directions carefully for loading the cartridge into the pen.

Injecting the Dose:

1. Wash your hands.
2. Use an alcohol swab to wipe the exposed rubber surface on the metal cap end of the cartridge or prefilled pen.
3. Inspect the HUMALOG in the cartridge. It should look clear and colourless. Do not use HUMALOG if it appears cloudy, thickened, or slightly coloured or if solid particles are visible.
4. Follow pen manufacturer's directions for attaching needle.
5. Hold the pen with needle pointing straight up. If there are large bubbles, tap the side of the pen until they float to the top. Remove the bubbles and the air in the needle by setting the pen to a 2-unit dose and depressing the plunger. Repeat this step if necessary until a drop of HUMALOG appears at the end of the needle.

6. To avoid tissue damage (skin thinning, skin thickening, or skin lumps), injection sites can be rotated so that the same site is not used more than approximately once a month.
7. Prepare the injection site as directed by your healthcare professional.
8. Insert the needle as instructed by your doctor.
9. To inject HUMALOG, follow the pen manufacturer's instructions.
10. Pull the needle out and apply gentle pressure over the injection site for several seconds. Do not rub the area.
11. Immediately after an injection, remove the needle from the pen. This will guard against contamination and prevent leakage, re-entry of air, and potential needle clogs. Dispose of the needle in a closable, puncture-resistant sharps container (like a biohazard container) or as directed by your healthcare professional. Do not reuse needle. **NEEDLES, CARTRIDGES, AND PENS MUST NOT BE SHARED.** To prevent the possible transmission of disease, never share a HUMALOG pen or cartridge between patients, even if the needle on the delivery device is changed.
12. Use the gauge on the side of the 3 mL cartridge to help you judge how much HUMALOG remains. The distance between each mark is approximately 20 units for 3 mL cartridges. When the leading edge of the plunger reaches the last mark on the gauge there is approximately 20 units of HUMALOG remaining in the cartridge. You may continue to use the cartridge until the plunger will no longer advance. See injection instructions accompanying the pen to ensure that a complete dose is obtained.

Usual dose

Your doctor has told you which insulin to use, how much, and when and how often to inject it. Because each patient's case of diabetes is different, this schedule has been individualized for you.

Your usual HUMALOG dose may be affected by changes in your food, activity, or work schedule. Carefully follow your doctor's instructions to allow for these changes. Other things that may affect your HUMALOG dose are illness, pregnancy, medication, exercise and travel.

Overdose

Hypoglycemia (too little glucose in the blood) is one of the most frequent adverse events experienced by insulin users. It can be brought about by:

1. Missing or delaying meals
2. Taking too much insulin
3. Exercising or working more than usual
4. An infection or illness (especially with diarrhea or vomiting)
5. A change in the body's need for insulin
6. Diseases of the adrenal, pituitary, or thyroid gland, or progression of kidney or liver disease

7. Interactions with other drugs that lower blood glucose, such as oral hypoglycemics, salicylates, sulfa antibiotics, and certain antidepressants
8. Consumption of alcoholic beverages

Dietary Implications:

If a usual meal cannot be obtained at the appropriate time, then to avoid hypoglycemia, you should take the amount of carbohydrate prescribed for this meal in the form of orange juice, syrup, candy, or bread and milk, without changing your insulin dosage. If it becomes necessary to omit a meal on account of nausea and vomiting, you should test your blood sugar level and notify your doctor.

Mild to moderate hypoglycemia may be treated by eating foods or drinks that contain sugar. Patients should always carry a quick source of sugar, such as candy mints or glucose tablets. More severe hypoglycemia may require the assistance of another person. Patients who are unable to take sugar orally or who are unconscious should be treated with intravenous administration of glucose at a medical facility or should be given an injection of glucagon (either intramuscular or subcutaneous). The patient should be given oral carbohydrates as soon as consciousness is recovered.

In case of drug overdose, contact a healthcare practitioner, hospital emergency department or regional Poison Control Centre immediately, even if there are no symptoms.

SIDE EFFECTS AND WHAT TO DO ABOUT THEM

Hypoglycemia:

One of the most frequent adverse events experienced by insulin users is hypoglycemia (see PROPER USE OF THIS MEDICATION).

Diabetic Acidosis and Coma:

Diabetic acidosis may develop if your body has too little insulin (this is the opposite of insulin reaction, which is the result of too much insulin in the blood). Diabetic acidosis may be brought on if you omit your insulin or take less than the doctor has prescribed, eat significantly more than your diet calls for, or develop a fever or infection. With acidosis, urine tests show a large amount of sugar and acetone.

The first symptoms of diabetic acidosis usually come on gradually, over a period of hours or days, and include a drowsy feeling, flushed face, thirst, and loss of appetite. Heavy breathing and a rapid pulse are more severe symptoms.

If uncorrected, loss of consciousness, coma, or death can result. Therefore, it is important that you obtain medical assistance immediately.

Lipoatrophy, Lipohypertrophy, or Localized Cutaneous Amyloidosis:

Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the skin), lipohypertrophy

(enlargement or thickening of tissue), or localized cutaneous amyloidosis (skin lumps). If you notice any of these conditions, consult your doctor. A change in your injection technique may help alleviate the problem.

Allergy to Insulin:

Patients occasionally experience redness, swelling, and itching at the site of injection of insulin. This condition, called local allergy, usually clears up in a few days to a few weeks. If you have local reactions, contact your doctor, who may recommend a change in the type or species of insulin.

Less common, but potentially more serious, is generalized allergy to insulin, which may cause rash over the whole body, shortness of breath, wheezing, reduction in blood pressure, fast pulse, or sweating. Severe cases of generalized allergy may be life threatening. If you think you are having a generalized allergic reaction to insulin, notify a doctor immediately. Your doctor may recommend skin testing, that is, injecting small doses of other insulins into the skin, in order to select the best insulin for you to use. Patients who have had severe generalized allergic reactions to insulin should be skin tested with each new preparation to be used before treatment with that preparation is started.

This is not a complete list of side effects. For any unexpected effects while taking HUMALOG, contact your doctor or pharmacist.

HOW TO STORE IT

Prior to first use, HUMALOG insulin cartridges or prefilled pens should be stored in a refrigerator between 2° and 8°C. Do not freeze. Do not expose to excessive heat or sunlight. The pen and cartridge of HUMALOG that you are currently using should not be refrigerated but should be kept as cool as possible (below 30°C) and away from direct heat and light. Do not use HUMALOG if it has been frozen. Cartridges or prefilled pens in use, or not refrigerated, should be discarded after 28 days, even if they still contain HUMALOG.

Inspection of Cartridge:

HUMALOG should be clear and colourless. DO NOT USE a cartridge or KwikPen of HUMALOG if it appears cloudy, thickened, or slightly coloured, or if solid particles are visible. A cartridge or KwikPen that is not clear and colourless or that is cracked or broken should be returned to the place of purchase for exchange.

If you notice anything unusual in the appearance or effect of your insulin, consult your healthcare professional.

DO NOT USE A CARTRIDGE OR PREFILLED PEN OF HUMALOG AFTER THE EXPIRATION DATE STAMPED ON THE LABEL.

Dispose of used needles in a puncture-resistant container or as directed by your healthcare professional.

Dispose of used pens as instructed by your healthcare professional and without the needle attached.

REPORTING SUSPECTED SIDE EFFECTS

You can report any suspected adverse reactions associated with the use of health products to the Canada Vigilance Program by one of the following 3 ways:

- Report online at www.healthcanada.gc.ca/medeffect
- Call toll-free at 1-866-234-2345
- Complete a Canada Vigilance Reporting Form and:
 - Fax toll-free to 1-866-678-6789, or
 - Mail to:
 - Canada Vigilance Program
 - Health Canada
 - Postal Locator 0701D
 - Ottawa, Ontario
 - K1A 0K9

Postage paid labels, Canada Vigilance Reporting Form and the adverse reaction reporting guidelines are available on the MedEffect™ Canada Web site at www.healthcanada.gc.ca/medeffect

NOTE: Should you require information related to the management of side effects, contact your health professional. The Canada Vigilance Program does not provide medical advice.

MORE INFORMATION

For more information, please contact your healthcare professionals or pharmacist first, or Eli Lilly Canada Inc. at:

1-888-545-5972 or visit the website at www.lilly.ca.

The information in this document is current as of the last revision date shown below. For the most current information please visit our website or contact us directly.

This leaflet was prepared by Eli Lilly Canada Inc.

HUMALOG, MIX25, MIX50 and KwikPen are registered trademarks owned by Eli Lilly and Company, its subsidiaries or affiliates.

You may need to read this package insert again. Please do not throw it away until you have finished your medicine.

Last revised: Month DD, 2021

LOG-0003-CA-PMI-2021MMDD

PART III: CONSUMER INFORMATION

HUMALOG® MIX25® CARTRIDGES

(25% insulin lispro injection, 75% insulin lispro protamine suspension)

Suspension for Injection, 100 units/mL, Lilly Standard

and HUMALOG® MIX25® KWIKPEN®

(25% insulin lispro injection, 75% insulin lispro protamine suspension)

Suspension for Injection, 100 units/mL, Lilly Standard

This leaflet is part III of a three-part "Product Monograph" published when HUMALOG® MIX25® was approved for sale in Canada and is designed specifically for Consumers. This leaflet is a summary and will not tell you everything about HUMALOG® MIX25®. Contact your doctor or pharmacist if you have any questions about the drug.

ABOUT THIS MEDICATION

What the medication is used for:

Insulin is a hormone produced by the pancreas, a large gland that lies near the stomach. This hormone is necessary for the body's correct use of food, especially sugar. Diabetes occurs when the pancreas does not make enough insulin to meet your body's needs.

To control your diabetes, your doctor has prescribed injections of insulin to keep your blood glucose at a near-normal level.

What it does:

Insulin lispro is a recombinant DNA sourced human insulin analogue. HUMALOG MIX25 is a mixture of fast-acting (insulin lispro) and long-acting (insulin lispro protamine) man-made insulins. HUMALOG MIX25 is used to control high blood sugar (glucose) in people with diabetes. HUMALOG MIX25 takes effect more rapidly and has a shorter duration of activity as compared to regular insulin.

The rapid onset of activity requires HUMALOG MIX25 to be given within 15 minutes before a meal. The time course of action of any insulin may vary to some extent in different individuals or at different times in the same individual. As with all insulin preparations, the duration of action of HUMALOG MIX25 is dependent on dose, site of injection, blood supply, temperature, and physical activity.

Proper control is important. Uncontrolled diabetes (hyperglycemia) over a long period of time can result in a number of serious problems such as blindness, kidney failure, poor circulation/heart attacks, strokes and/or nerve damage. These problems can be prevented or reduced by good diabetes management. This will require close and constant cooperation with your diabetes healthcare team including: yourself, your doctor and your diabetes educators (nurses, dietitians, social workers, pharmacists and other healthcare professionals). Thus, you can lead an active, healthy and productive life by eating a

balanced daily diet, exercising regularly, and taking your insulin injections as prescribed.

You have been instructed to test your blood and/or your urine regularly for glucose. If your blood tests consistently show above- or below-normal glucose levels or your urine tests consistently show the presence of glucose, your diabetes is not properly controlled and you must let your doctor know.

When it should not be used:

- When your blood sugar is too low (hypoglycemia). After treating your low blood sugar, follow your healthcare provider's instructions on the use of HUMALOG MIX25 insulin.
- If you are allergic to anything in HUMALOG MIX25. A complete list of ingredients in HUMALOG MIX25 insulin is provided below.

What the medicinal ingredient is:

HUMALOG MIX25 insulin contains 100 units/mL of Human Insulin Analogue.

HUMALOG MIX25 contains a mix of insulin lispro injection (25%) and insulin lispro protamine suspension (75%).

What the non-medicinal ingredients are:

HUMALOG MIX25 contains glycerol, dibasic sodium phosphate, m-cresol, zinc (as ion) and water for injection. Hydrochloric acid or sodium hydroxide may be added to adjust pH. HUMALOG MIX25 also contains liquefied phenol, protamine sulphate, and zinc oxide.

What dosage forms it comes in:

HUMALOG MIX25 is a sterile suspension containing 25% insulin lispro injection and 75% insulin lispro protamine suspension. It is available in:

- Cartridge, 3 mL
- KwikPen, 3 mL prefilled pen

Other HUMALOG products include:

- HUMALOG 100 units/mL (insulin lispro injection)
- HUMALOG 200 units/mL KwikPen (insulin lispro injection)
- HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension)

HUMALOG MIX25 prefilled pens and cartridges are available in boxes of 5. HUMALOG MIX25 cartridges are designed for use with Lilly injector systems. The cartridge or prefilled pen containing HUMALOG MIX25 is not designed to allow any other insulin to be mixed in the cartridge or for the cartridge or prefilled pen to be reused.

For guidance on the use of the Pen (prefilled, disposable insulin injector), please refer to the separate Instructions for Use enclosed within the packaging.

DO NOT USE ANY OTHER INSULIN EXCEPT ON YOUR DOCTOR'S ADVICE AND DIRECTION.

Always keep an extra supply of HUMALOG MIX25 i.e. a spare pen and cartridge or prefilled pen on hand. Always wear identification to indicate that you have diabetes so that appropriate treatment can be given if complications occur away from home.

When you receive your insulin from the pharmacy, always check to see that:

1. The name HUMALOG MIX25 appears on the carton and cartridge or prefilled pen label.
2. The carton and cartridge or prefilled pen label is correct for your type of insulin.
3. The insulin strength is U-100.
4. The expiration date on the package will allow you to use the insulin before that date.

WARNINGS AND PRECAUTIONS

Serious Warnings and Precautions

- Hypoglycemia or low blood sugar is the most common adverse effect experienced by insulin users. Blood glucose monitoring is recommended for all patients with diabetes. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma or even death. Information on how to recognize these symptoms is provided below.
- This Lilly human insulin analogue differs from other insulins because it has a unique structure, a very quick onset of action and a short duration of activity. HUMALOG MIX25 should be given within 15 minutes before a meal.
- HUMALOG MIX25 is a white suspension and should be administered by subcutaneous injection only. HUMALOG MIX25 must not be administered intravenously.
- Any change of insulin regimen should be made cautiously and only under medical supervision. Changes in purity, strength, brand (manufacturer), type (regular, NPH, etc), species (beef, pork, beef-pork, human), and/or method of manufacture (recombinant DNA versus animal-source insulin) may result in the need for a change in dosage.
- Mixing of HUMALOG MIX25 with either animal insulins or insulin preparations produced by other manufacturers is not recommended.
- Patients taking HUMALOG MIX25 may require a change in dosage from that used with other insulins. If an adjustment is needed, it may occur with the first dose or over a period of several weeks.

BEFORE you use HUMALOG MIX25 talk to your doctor or pharmacist if:

- You have trouble with your kidneys or liver, your doctor may decide to alter your insulin dose.

- You drink alcohol (including wine and beer): watch for signs of hypoglycemia and never drink alcohol on an empty stomach.
- You exercise more than usual or if you want to change your usual diet. Exercise may lower your body's need for insulin during and for some time after the activity. Exercise may also speed up the effect of an insulin dose, especially if the exercise involves the area of injection site.
- You are ill. Illness, especially with nausea and vomiting, may cause your insulin requirements to change. Even if you are not eating, you will still require insulin. You and your doctor should establish a sick day plan for you to use in case of illness. When you are sick, test your blood/urine frequently.
- You are travelling across more than 2 time zones. You should consult your doctor concerning adjustments in your insulin schedule.
- You are pregnant. HUMALOG MIX25 can be used in pregnancy if clinically indicated. Data on a large number of exposed pregnancies do not indicate any adverse effect of HUMALOG MIX25 on pregnancy or on the health of the foetus/newborn. Good control of diabetes is especially important for you and your unborn baby. Pregnancy may make managing your diabetes more difficult. If you are planning to have a baby, are pregnant, or are nursing a baby, consult your doctor.
- When you use other medicines. Many medicines affect the way glucose works in your body and this may influence your insulin dose. Listed below are the most common medicines, which may affect your insulin treatment. Talk to your doctor or pharmacist if you take, or change any other medicines, even those not prescribed.

INTERACTIONS WITH THIS MEDICATION

Insulin requirements may be increased if you are taking other drugs with hyperglycemic activity, such as oral contraceptives (for example, birth control pills, injections and patches), corticosteroids, or thyroid replacement therapy. Insulin requirements may be decreased in the presence of agents such as oral antidiabetic agents, salicylates (aspirin), sulfa antibiotics, certain antidepressants (monoamine oxidase inhibitors), beta-blockers, alcohol, ACE-inhibitors and angiotensin II receptor blockers. Always discuss any medications you are taking with your doctor.

The use of thiazolidinediones (such as rosiglitazone and pioglitazone), alone or in combination with other antidiabetic agents (including insulin), has been associated with heart failure and swelling of the lower extremities. Please contact your physician immediately if you develop symptoms of shortness of breath, fatigue, exercise intolerance, or swelling of the lower extremities while you are on these agents.

PROPER USE OF THIS MEDICATION

HUMALOG MIX25

The 3 mL cartridge is only for use in 3 mL pens.

Preparing a Cartridge of HUMALOG MIX25 for Insertion in a Pen

1. Wash your hands.
2. Cartridges containing HUMALOG MIX25 should be rotated in the palms of the hands ten times and inverted 180° ten times immediately before use to resuspend insulin until it appears uniformly cloudy or milky. If not, repeat the above procedure until contents are mixed. Cartridges contain a small glass bead to assist mixing. Do not shake vigorously as this may cause frothing which may interfere with the correct measurement of the dose.
3. Inspect HUMALOG MIX25 cartridge before inserting it into the pen. Do not use the HUMALOG MIX25 cartridge if clumps of material are present or if solid white particles stick to the bottom or wall of the cartridge, giving it a frosted appearance or if the cartridge is cracked or broken.
4. Follow the pen manufacturer's directions carefully for loading the cartridge into the pen.

Injecting the Dose:

1. Wash your hands.
2. Use an alcohol swab to wipe the exposed rubber surface on the metal cap end of the cartridge or prefilled pen.
3. Inspect the HUMALOG MIX25 in the cartridge. It should look uniformly cloudy or milky.
4. Follow pen manufacturer's directions for attaching needle.
5. Hold the pen with needle pointing straight up. If there are large bubbles, tap the side of the pen until they float to the top. Remove the bubbles and the air in the needle by setting the pen to a 2-unit dose and depressing the plunger. Repeat this step if necessary until a drop of HUMALOG MIX25 appears at the end of the needle.
6. To avoid tissue damage (skin thinning, skin thickening, or skin lumps), injection sites can be rotated so that the same site is not used more than approximately once a month.
7. Prepare the injection site as directed by your healthcare professional.
8. Insert the needle as instructed by your doctor.
9. To inject HUMALOG MIX25, follow the pen manufacturer's instructions.
10. Pull the needle out and apply gentle pressure over the injection site for several seconds. Do not rub the area.
11. Immediately after an injection, remove the needle from the pen. This will guard against contamination and prevent leakage, re-entry of air, and potential needle clogs. Dispose of the needle in a closable, puncture-resistant sharps container (like a biohazard container) or as directed by your healthcare professional. Do not reuse needle. **NEEDLES, CARTRIDGES, AND PENS MUST NOT BE SHARED.** To prevent the possible transmission of disease, never share a HUMALOG MIX25 pen or cartridge between patients, even if the needle on the delivery device is changed.

12. Use the gauge on the side of the 3 mL cartridge to help you judge how much HUMALOG MIX25 remains once it is in use. The distance between each mark is approximately 20 units for 3 mL cartridges. When the leading edge of the plunger reaches the last mark on the gauge there is approximately 20 units of HUMALOG MIX25 remaining in the cartridge. You may continue to use the cartridge until the plunger will no longer advance. See injection instructions accompanying the pen to ensure that a complete dose is obtained.

Usual dose

Your doctor has told you which insulin to use, how much, and when and how often to inject it. Because each patient's case of diabetes is different, this schedule has been individualized for you.

Your usual HUMALOG MIX25 dose may be affected by changes in your food, activity, or work schedule. Carefully follow your doctor's instructions to allow for these changes. Other things that may affect your HUMALOG MIX25 dose are illness, pregnancy, medication, exercise and travel.

Overdose

Hypoglycemia (too little glucose in the blood) is one of the most frequent adverse events experienced by insulin users. It can be brought about by:

1. Missing or delaying meals
2. Taking too much insulin
3. Exercising or working more than usual
4. An infection or illness (especially with diarrhea or vomiting)
5. A change in the body's need for insulin
6. Diseases of the adrenal, pituitary, or thyroid gland, or progression of kidney or liver disease
7. Interactions with other drugs that lower blood glucose, such as oral hypoglycemics, salicylates, sulfa antibiotics, and certain antidepressants
8. Consumption of alcoholic beverages

Dietary Implications:

If a usual meal cannot be obtained at the appropriate time, then to avoid hypoglycemia, you should take the amount of carbohydrate prescribed for this meal in the form of orange juice, syrup, candy, or bread and milk, without changing your insulin dosage. If it becomes necessary to omit a meal on account of nausea and vomiting, you should test your blood sugar level and notify your doctor.

Mild to moderate hypoglycemia may be treated by eating foods or drinks that contain sugar. Patients should always carry a quick source of sugar, such as candy mints or glucose tablets. More severe hypoglycemia may require the assistance of another person. Patients who are unable to take sugar orally or who are unconscious should be treated with intravenous administration of glucose at a medical facility or should be given an injection of glucagon (either

intramuscular or subcutaneous). The patient should be given oral carbohydrates as soon as consciousness is recovered.

In case of drug overdose, contact a healthcare practitioner, hospital emergency department or regional Poison Control Centre immediately, even if there are no symptoms.

SIDE EFFECTS AND WHAT TO DO ABOUT THEM

Hypoglycemia:

One of the most frequent adverse events experienced by insulin users is hypoglycaemia (see PROPER USE OF THIS MEDICATION).

Diabetic Acidosis and Coma:

Diabetic acidosis may develop if your body has too little insulin (this is the opposite of insulin reaction, which is the result of too much insulin in the blood). Diabetic acidosis may be brought on if you omit your insulin or take less than the doctor has prescribed, eat significantly more than your diet calls for, or develop a fever or infection. With acidosis, urine tests show a large amount of sugar and acetone.

The first symptoms of diabetic acidosis usually come on gradually, over a period of hours or days, and include a drowsy feeling, flushed face, thirst, and loss of appetite. Heavy breathing and a rapid pulse are more severe symptoms.

If uncorrected, loss of consciousness, coma, or death can result. Therefore, it is important that you obtain medical assistance immediately.

Lipoatrophy, Lipohypertrophy, or Localized Cutaneous Amyloidosis:

Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the skin), lipohypertrophy (enlargement or thickening of tissue), or localized cutaneous amyloidosis (skin lumps). If you notice any of these conditions, consult your doctor. A change in your injection technique may help alleviate the problem.

Allergy to Insulin:

Patients occasionally experience redness, swelling, and itching at the site of injection of insulin. This condition, called local allergy, usually clears up in a few days to a few weeks. If you have local reactions, contact your doctor, who may recommend a change in the type or species of insulin.

Less common, but potentially more serious, is generalized allergy to insulin, which may cause rash over the whole body, shortness of breath, wheezing, reduction in blood pressure, fast pulse, or sweating. Severe cases of generalized allergy may be life threatening. If you think you are having a generalized allergic reaction to insulin, notify a doctor immediately. Your doctor may recommend skin testing, that is, injecting small doses of other insulins into the skin, in order to select the best insulin for you to use. Patients who have had severe generalized allergic reactions to insulin should be skin tested with each new

preparation to be used before treatment with that preparation is started.

This is not a complete list of side effects. For any unexpected effects while taking HUMALOG MIX25, contact your doctor or pharmacist.

HOW TO STORE IT

Prior to first use, HUMALOG MIX25 cartridges or prefilled pens should be stored in a refrigerator between 2° and 8°C. Do not freeze. Do not expose to excessive heat or sunlight. The pen and cartridge of HUMALOG MIX25 that you are currently using should not be refrigerated but should be kept as cool as possible (below 30°C) and away from direct heat and light. Do not use HUMALOG MIX25 if it has been frozen. Cartridges or prefilled pens in use, or not refrigerated, should be discarded after 28 days, even if they still contain HUMALOG MIX25.

Inspection of Cartridge:

DO NOT USE a cartridge or KwikPen of HUMALOG MIX25 if clumps of material are present or if solid white particles stick to the bottom or wall of the cartridge, giving it a frosted appearance. A cartridge or KwikPen that is cracked or broken should be returned to the place of purchase for exchange.

If you notice anything unusual in the appearance or effect of your insulin, consult your healthcare professional.

DO NOT USE A CARTRIDGE OR PREFILLED PEN OF HUMALOG MIX25 AFTER THE EXPIRATION DATE STAMPED ON THE LABEL. Dispose of used needles in a puncture-resistant container or as directed by your healthcare professional.

Dispose of used pens as instructed by your healthcare professional and without the needle attached.

REPORTING SUSPECTED SIDE EFFECTS

You can report any suspected adverse reactions associated with the use of health products to the Canada Vigilance Program by one of the following 3 ways:

- Report online at www.healthcanada.gc.ca/medeffect
- Call toll-free at 1-866-234-2345
- Complete a Canada Vigilance Reporting Form and:
 - Fax toll-free to 1-866-678-6789, or
 - Mail to:
 - Canada Vigilance Program
 - Health Canada
 - Postal Locator 0701D
 - Ottawa, Ontario
 - K1A 0K9

Postage paid labels, Canada Vigilance Reporting Form and the adverse reaction reporting guidelines are available on the MedEffect™ Canada Web site at www.healthcanada.gc.ca/medeffect

NOTE: Should you require information related to the management of side effects, contact your health professional. The Canada Vigilance Program does not provide medical advice.

MORE INFORMATION

For more information, please contact your healthcare professionals or pharmacist first, or Eli Lilly Canada Inc. at:

1-888-545-5972 or visit the website at www.lilly.ca.

The information in this document is current as of the last revision date shown below. For the most current information please visit our website or contact us directly.

This leaflet was prepared by Eli Lilly Canada Inc.

HUMALOG, MIX25, MIX50 and KwikPen are registered trademarks owned by Eli Lilly and Company, its subsidiaries or affiliates.

You may need to read this package insert again. Please do not throw it away until you have finished your medicine.

Last revised: Month DD, 2021

LOG7525-0002-CA-PMI-2021MMDD

PART III: CONSUMER INFORMATION

HUMALOG MIX50® CARTRIDGES

(50% insulin lispro injection, 50% insulin lispro protamine suspension)

Suspension for Injection, 100 units/mL, Lilly Standard

and HUMALOG MIX50® KWIKPEN®

(50% insulin lispro injection, 50% insulin lispro protamine suspension)

Suspension for Injection, 100 units/mL, Lilly Standard

This leaflet is part III of a three-part "Product Monograph" published when HUMALOG MIX50® was approved for sale in Canada and is designed specifically for Consumers. This leaflet is a summary and will not tell you everything about HUMALOG MIX50®. Contact your doctor or pharmacist if you have any questions about the drug.

ABOUT THIS MEDICATION

What the medication is used for:

Insulin is a hormone produced by the pancreas, a large gland that lies near the stomach. This hormone is necessary for the body's correct use of food, especially sugar. Diabetes occurs when the pancreas does not make enough insulin to meet your body's needs.

To control your diabetes, your doctor has prescribed injections of insulin to keep your blood glucose at a near-normal level.

What it does:

Insulin lispro is a recombinant DNA sourced human insulin analogue. HUMALOG MIX50 is a mixture of fast-acting (insulin lispro) and long-acting (insulin lispro protamine) man-made insulins. HUMALOG MIX50 is used to control high blood sugar (glucose) in people with diabetes. HUMALOG MIX50 takes effect more rapidly and has a shorter duration of activity as compared to regular insulin.

The rapid onset of activity requires HUMALOG MIX50 to be given within 15 minutes before a meal. The time course of action of any insulin may vary to some extent in different individuals or at different times in the same individual. As with all insulin preparations, the duration of action of HUMALOG MIX50 is dependent on dose, site of injection, blood supply, temperature, and physical activity.

Proper control is important. Uncontrolled diabetes (hyperglycemia) over a long period of time can result in a number of serious problems such as blindness, kidney failure, poor circulation/heart attacks, strokes and/or nerve damage. These problems can be prevented or reduced by good diabetes management. This will require close and constant cooperation with your diabetes healthcare team including: yourself, your doctor and your diabetes educators (nurses, dietitians, social workers, pharmacists and other healthcare professionals). Thus, you can lead an active, healthy and productive life by eating a

balanced daily diet, exercising regularly, and taking your insulin injections as prescribed.

You have been instructed to test your blood and/or your urine regularly for glucose. If your blood tests consistently show above- or below-normal glucose levels or your urine tests consistently show the presence of glucose, your diabetes is not properly controlled and you must let your doctor know.

When it should not be used:

- When your blood sugar is too low (hypoglycemia). After treating your low blood sugar, follow your healthcare provider's instructions on the use of HUMALOG MIX50 insulin.
- If you are allergic to anything in HUMALOG MIX50. A complete list of ingredients in HUMALOG MIX50 insulin is provided below.

What the medicinal ingredient is:

HUMALOG MIX50 insulin contains 100 units/mL of Human Insulin Analogue.

HUMALOG MIX50 contains a mix of insulin lispro injection (50%) and insulin lispro protamine suspension (50%).

What the non-medicinal ingredients are:

HUMALOG MIX50 contains glycerol, dibasic sodium phosphate, m-cresol, zinc (as ion) and water for injection. Hydrochloric acid or sodium hydroxide may be added to adjust pH. HUMALOG MIX50 also contains liquefied phenol, protamine sulphate, and zinc oxide.

What dosage forms it comes in:

HUMALOG MIX50 is a sterile suspension containing 50% insulin lispro injection and 50% insulin lispro protamine suspension. It is available in:

- Cartridge, 3 mL
- KwikPen, 3 mL prefilled pen

Other HUMALOG products include:

- HUMALOG 100 units/mL (insulin lispro injection)
- HUMALOG 200 units/mL KwikPen (insulin lispro injection)
- HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension)

HUMALOG MIX50 prefilled pens and cartridges are available in boxes of 5. HUMALOG MIX50 cartridges are designed for use with Lilly injector systems. The cartridge or prefilled pen containing HUMALOG MIX50 is not designed to allow any other insulin to be mixed in the cartridge or for the cartridge or prefilled pen to be reused.

For guidance on the use of the Pen (prefilled, disposable insulin injector), please refer to the separate Instructions for Use enclosed within the packaging.

DO NOT USE ANY OTHER INSULIN EXCEPT ON YOUR DOCTOR'S ADVICE AND DIRECTION.

Always keep an extra supply of HUMALOG MIX50 i.e. a spare pen and cartridge or prefilled pen on hand. Always wear identification to indicate that you have diabetes so that appropriate treatment can be given if complications occur away from home.

When you receive your insulin from the pharmacy, always check to see that:

1. The name HUMALOG MIX50 appears on the carton and cartridge or prefilled pen label.
2. The carton and cartridge or prefilled pen label is correct for your type of insulin.
3. The insulin strength is U-100.
4. The expiration date on the package will allow you to use the insulin before that date.

WARNINGS AND PRECAUTIONS

Serious Warnings and Precautions

- Hypoglycemia or low blood sugar is the most common adverse effect experienced by insulin users. Blood glucose monitoring is recommended for all patients with diabetes. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma or even death. Information on how to recognize these symptoms is provided below.
- This Lilly human insulin analogue differs from other insulins because it has a unique structure, a very quick onset of action and a short duration of activity. HUMALOG MIX50 should be given within 15 minutes before a meal.
- HUMALOG MIX50 is a white suspension and should be administered by subcutaneous injection only. HUMALOG MIX50 must not be administered intravenously.
- Any change of insulin regimen should be made cautiously and only under medical supervision. Changes in purity, strength, brand (manufacturer), type (regular, NPH, etc), species (beef, pork, beef-pork, human), and/or method of manufacture (recombinant DNA versus animal-source insulin) may result in the need for a change in dosage.
- Mixing of HUMALOG MIX50 with either animal insulins or insulin preparations produced by other manufacturers is not recommended.
- Patients taking HUMALOG MIX50 may require a change in dosage from that used with other insulins. If an adjustment is needed, it may occur with the first dose or over a period of several weeks.

BEFORE you use HUMALOG MIX50 talk to your doctor or pharmacist if:

- You have trouble with your kidneys or liver, your doctor may decide to alter your insulin dose.

- You drink alcohol (including wine and beer): watch for signs of hypoglycemia and never drink alcohol on an empty stomach.
- You exercise more than usual or if you want to change your usual diet. Exercise may lower your body's need for insulin during and for some time after the activity. Exercise may also speed up the effect of an insulin dose, especially if the exercise involves the area of injection site.
- You are ill. Illness, especially with nausea and vomiting, may cause your insulin requirements to change. Even if you are not eating, you will still require insulin. You and your doctor should establish a sick day plan for you to use in case of illness. When you are sick, test your blood/urine frequently.
- You are travelling across more than 2 time zones. You should consult your doctor concerning adjustments in your insulin schedule.
- You are pregnant. HUMALOG MIX50 can be used in pregnancy if clinically indicated. Data on a large number of exposed pregnancies do not indicate any adverse effect of HUMALOG MIX50 on pregnancy or on the health of the foetus/newborn. Good control of diabetes is especially important for you and your unborn baby. Pregnancy may make managing your diabetes more difficult. If you are planning to have a baby, are pregnant, or are nursing a baby, consult your doctor.
- When you use other medicines. Many medicines affect the way glucose works in your body and this may influence your insulin dose. Listed below are the most common medicines, which may affect your insulin treatment. Talk to your doctor or pharmacist if you take, or change any other medicines, even those not prescribed.

INTERACTIONS WITH THIS MEDICATION

Insulin requirements may be increased if you are taking other drugs with hyperglycemic activity, such as oral contraceptives (for example, birth control pills, injections and patches), corticosteroids, or thyroid replacement therapy. Insulin requirements may be decreased in the presence of agents such as oral antidiabetic agents, salicylates (aspirin), sulfa antibiotics, certain antidepressants (monoamine oxidase inhibitors), beta-blockers, alcohol, ACE-inhibitors and angiotensin II receptor blockers. Always discuss any medications you are taking with your doctor.

The use of thiazolidinediones (such as rosiglitazone and pioglitazone), alone or in combination with other antidiabetic agents (including insulin), has been associated with heart failure and swelling of the lower extremities. Please contact your physician immediately if you develop symptoms of shortness of breath, fatigue, exercise intolerance, or swelling of the lower extremities while you are on these agents.

PROPER USE OF THIS MEDICATION

HUMALOG MIX50

The 3 mL cartridge is only for use in 3 mL pens.

Preparing a Cartridge of HUMALOG MIX50 for Insertion in a Pen

1. Wash your hands.
2. Cartridges containing HUMALOG MIX50 should be rotated in the palms of the hands ten times and inverted 180° ten times immediately before use to resuspend insulin until it appears uniformly cloudy or milky. If not, repeat the above procedure until contents are mixed. Cartridges contain a small glass bead to assist mixing. Do not shake vigorously as this may cause frothing which may interfere with the correct measurement of the dose.
3. Inspect HUMALOG MIX50 cartridge before inserting it into the pen. Do not use the HUMALOG MIX50 cartridge if clumps of material are present or if solid white particles stick to the bottom or wall of the cartridge, giving it a frosted appearance or if the cartridge is cracked or broken.
4. Follow the pen manufacturer's directions carefully for loading the cartridge into the pen.

Injecting the Dose:

1. Wash your hands.
2. Use an alcohol swab to wipe the exposed rubber surface on the metal cap end of the cartridge or prefilled pen.
3. Inspect the HUMALOG MIX50 in the cartridge. It should look uniformly cloudy or milky.
4. Follow pen manufacturer's directions for attaching needle.
5. Hold the pen with needle pointing straight up. If there are large bubbles, tap the side of the pen until they float to the top. Remove the bubbles and the air in the needle by setting the pen to a 2-unit dose and depressing the plunger. Repeat this step if necessary until a drop of HUMALOG MIX50 appears at the end of the needle.
6. To avoid tissue damage (skin thinning, skin thickening, or skin lumps), injection sites can be rotated so that the same site is not used more than approximately once a month.
7. Prepare the injection site as directed by your healthcare professional.
8. Insert the needle as instructed by your doctor.
9. To inject HUMALOG MIX50, follow the pen manufacturer's instructions.
10. Pull the needle out and apply gentle pressure over the injection site for several seconds. Do not rub the area.
11. Immediately after an injection, remove the needle from the pen. This will guard against contamination and prevent leakage, re-entry of air, and potential needle clogs. Dispose of the needle in a closable, puncture-resistant sharps container (like a biohazard container) or as directed by your healthcare professional. Do not reuse needle. **NEEDLES, CARTRIDGES, AND PENS MUST NOT BE SHARED.** To prevent the possible transmission of disease, never share a HUMALOG MIX50 pen or cartridge between patients, even if the needle on the delivery device is changed.

12. Use the gauge on the side of the 3 mL cartridge to help you judge how much HUMALOG MIX50 remains once it is in use. The distance between each mark is approximately 20 units for 3 mL cartridges. When the leading edge of the plunger reaches the last mark on the gauge there is approximately 20 units of HUMALOG MIX50 remaining in the cartridge. You may continue to use the cartridge until the plunger will no longer advance. See injection instructions accompanying the pen to ensure that a complete dose is obtained.

Usual dose

Your doctor has told you which insulin to use, how much, and when and how often to inject it. Because each patient's case of diabetes is different, this schedule has been individualized for you.

Your usual HUMALOG MIX50 dose may be affected by changes in your food, activity, or work schedule. Carefully follow your doctor's instructions to allow for these changes. Other things that may affect your HUMALOG MIX50 dose are illness, pregnancy, medication, exercise and travel.

Overdose

Hypoglycemia (too little glucose in the blood) is one of the most frequent adverse events experienced by insulin users. It can be brought about by:

1. Missing or delaying meals
2. Taking too much insulin
3. Exercising or working more than usual
4. An infection or illness (especially with diarrhea or vomiting)
5. A change in the body's need for insulin
6. Diseases of the adrenal, pituitary, or thyroid gland, or progression of kidney or liver disease
7. Interactions with other drugs that lower blood glucose, such as oral hypoglycemics, salicylates, sulfa antibiotics, and certain antidepressants
8. Consumption of alcoholic beverages

Dietary Implications:

If a usual meal cannot be obtained at the appropriate time, then to avoid hypoglycemia, you should take the amount of carbohydrate prescribed for this meal in the form of orange juice, syrup, candy, or bread and milk, without changing your insulin dosage. If it becomes necessary to omit a meal on account of nausea and vomiting, you should test your blood sugar level and notify your doctor.

Mild to moderate hypoglycemia may be treated by eating foods or drinks that contain sugar. Patients should always carry a quick source of sugar, such as candy mints or glucose tablets. More severe hypoglycemia may require the assistance of another person. Patients who are unable to take sugar orally or who are unconscious should be treated with intravenous administration of glucose at a medical facility or should be given an injection of glucagon (either

intramuscular or subcutaneous). The patient should be given oral carbohydrates as soon as consciousness is recovered.

In case of drug overdose, contact a healthcare practitioner, hospital emergency department or regional Poison Control Centre immediately, even if there are no symptoms.

SIDE EFFECTS AND WHAT TO DO ABOUT THEM

Hypoglycemia:

One of the most frequent adverse events experienced by insulin users is hypoglycaemia (see PROPER USE OF THIS MEDICATION).

Diabetic Acidosis and Coma:

Diabetic acidosis may develop if your body has too little insulin (this is the opposite of insulin reaction, which is the result of too much insulin in the blood). Diabetic acidosis may be brought on if you omit your insulin or take less than the doctor has prescribed, eat significantly more than your diet calls for, or develop a fever or infection. With acidosis, urine tests show a large amount of sugar and acetone.

The first symptoms of diabetic acidosis usually come on gradually, over a period of hours or days, and include a drowsy feeling, flushed face, thirst, and loss of appetite. Heavy breathing and a rapid pulse are more severe symptoms.

If uncorrected, loss of consciousness, coma, or death can result. Therefore, it is important that you obtain medical assistance immediately.

Lipoatrophy, Lipohypertrophy, or Localized Cutaneous Amyloidosis:

Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the skin), lipohypertrophy (enlargement or thickening of tissue), or localized cutaneous amyloidosis (skin lumps). If you notice any of these conditions, consult your doctor. A change in your injection technique may help alleviate the problem.

Allergy to Insulin:

Patients occasionally experience redness, swelling, and itching at the site of injection of insulin. This condition, called local allergy, usually clears up in a few days to a few weeks. If you have local reactions, contact your doctor, who may recommend a change in the type or species of insulin.

Less common, but potentially more serious, is generalized allergy to insulin, which may cause rash over the whole body, shortness of breath, wheezing, reduction in blood pressure, fast pulse, or sweating. Severe cases of generalized allergy may be life threatening. If you think you are having a generalized allergic reaction to insulin, notify a doctor immediately. Your doctor may recommend skin testing, that is, injecting small doses of other insulins into the skin, in order to select the best insulin for you to use. Patients who have had severe generalized allergic reactions to insulin should be skin tested with each new

preparation to be used before treatment with that preparation is started.

This is not a complete list of side effects. For any unexpected effects while taking HUMALOG MIX50, contact your doctor or pharmacist.

HOW TO STORE IT

Prior to first use, HUMALOG MIX50 cartridges or prefilled pens should be stored in a refrigerator between 2° and 8°C. Do not freeze. Do not expose to excessive heat or sunlight. The pen and cartridge of HUMALOG MIX50 that you are currently using should not be refrigerated but should be kept as cool as possible (below 30°C) and away from direct heat and light. Do not use HUMALOG MIX50 if it has been frozen. Cartridges or prefilled pens in use, or not refrigerated, should be discarded after 28 days, even if they still contain HUMALOG MIX50.

Inspection of Cartridge:

DO NOT USE a cartridge or KwikPen of HUMALOG MIX50 if clumps of material are present or if solid white particles stick to the bottom or wall of the cartridge, giving it a frosted appearance. A cartridge or KwikPen that is cracked or broken should be returned to the place of purchase for exchange.

If you notice anything unusual in the appearance or effect of your insulin, consult your healthcare professional.

DO NOT USE A CARTRIDGE OR PREFILLED PEN OF HUMALOG MIX50 AFTER THE EXPIRATION DATE STAMPED ON THE LABEL. Dispose of used needles in a puncture-resistant container or as directed by your healthcare professional.

Dispose of used pens as instructed by your healthcare professional and without the needle attached.

REPORTING SUSPECTED SIDE EFFECTS

You can report any suspected adverse reactions associated with the use of health products to the Canada Vigilance Program by one of the following 3 ways:

- Report online at www.healthcanada.gc.ca/medeffect
- Call toll-free at 1-866-234-2345
- Complete a Canada Vigilance Reporting Form and:
 - Fax toll-free to 1-866-678-6789, or
 - Mail to:
 - Canada Vigilance Program
 - Health Canada
 - Postal Locator 0701D
 - Ottawa, Ontario
 - K1A 0K9

Postage paid labels, Canada Vigilance Reporting Form and the adverse reaction reporting guidelines are available on the MedEffect™ Canada Web site at www.healthcanada.gc.ca/medeffect

NOTE: Should you require information related to the management of side effects, contact your health professional. The Canada Vigilance Program does not provide medical advice.

MORE INFORMATION

For more information, please contact your healthcare professionals or pharmacist first, or Eli Lilly Canada Inc. at:

1-888-545-5972 or visit the website at www.lilly.ca.

The information in this document is current as of the last revision date shown below. For the most current information please visit our website or contact us directly.

This leaflet was prepared by Eli Lilly Canada Inc.

HUMALOG, MIX25, MIX50 and KwikPen are registered trademarks owned by Eli Lilly and Company, its subsidiaries or affiliates.

You may need to read this package insert again. Please do not throw it away until you have finished your medicine.

Last revised: Month DD, 2021

LOG5050-0002-CA-PMI-2021MMDD

PART III: CONSUMER INFORMATION

HUMALOG® 200 units/mL KWIKPEN®
(insulin lispro injection)

Solution for Injection, 200 units/mL, Lilly Standard

This leaflet is part III of a three-part "Product Monograph" published when HUMALOG® was approved for sale in Canada and is designed specifically for Consumers. This leaflet is a summary and will not tell you everything about HUMALOG®. Contact your doctor or pharmacist if you have any questions about the drug.

ABOUT THIS MEDICATION

What the medication is used for:

Insulin is a hormone produced by the pancreas, a large gland that lies near the stomach. This hormone is necessary for the body's correct use of food, especially sugar. Diabetes occurs when the pancreas does not make enough insulin to meet your body's needs.

To control your diabetes, your doctor has prescribed injections of insulin to keep your blood glucose at a near-normal level.

What it does:

HUMALOG (insulin lispro) is a recombinant DNA sourced human insulin analogue. HUMALOG consists of zinc-insulin lispro crystals dissolved in a clear fluid. HUMALOG is used to control high blood sugar (glucose) in people with diabetes. HUMALOG takes effect more rapidly and has a shorter duration of activity as compared to regular insulin.

The rapid onset of activity requires HUMALOG to be given within 15 minutes before a meal. When necessary, HUMALOG may be given shortly after a meal instead (within 20 minutes of the start of the meal). The time course of action of any insulin may vary to some extent in different individuals or at different times in the same individual. As with all insulin preparations, the duration of action of HUMALOG is dependent on dose, site of injection, blood supply, temperature, and physical activity.

Proper control is important. Uncontrolled diabetes (hyperglycemia) over a long period of time can result in a number of serious problems such as blindness, kidney failure, poor circulation/heart attacks, strokes and/or nerve damage. These problems can be prevented or reduced by good diabetes management. This will require close and constant cooperation with your diabetes healthcare team including: yourself, your doctor and your diabetes educators (nurses, dietitians, social workers, pharmacists and other healthcare professionals). Thus, you can lead an active, healthy and productive life by eating a balanced daily diet, exercising regularly, and taking your insulin injections as prescribed.

You have been instructed to test your blood and/or your urine regularly for glucose. If your blood tests consistently show

above- or below-normal glucose levels or your urine tests consistently show the presence of glucose, your diabetes is not properly controlled and you must let your doctor know.

When it should not be used:

- When your blood sugar is too low (hypoglycemia). After treating your low blood sugar, follow your healthcare provider's instructions on the use of HUMALOG.
- If you are allergic to anything in HUMALOG. A complete list of ingredients in HUMALOG is provided below.
- With a syringe and needle or in a continuous subcutaneous insulin injection device (also known as insulin pump).

What the medicinal ingredient is:

HUMALOG 200 units/mL KwikPen contains 200 units/mL of Human Insulin Analogue.

HUMALOG contains insulin lispro injection.

What the non-medicinal ingredients are:

HUMALOG 200 units/mL contains glycerol, tromethamine, *m*-cresol, zinc oxide, and water for injection. Hydrochloric acid or sodium hydroxide may have been added to adjust pH.

What dosage forms it comes in:

HUMALOG 200 units/mL is a sterile solution containing insulin lispro injection. It is available in:

- KwikPen, 3 mL prefilled pen

Other HUMALOG products include:

- HUMALOG 100 units/mL (insulin lispro injection)
- HUMALOG MIX25 (25% insulin lispro injection, 75% insulin lispro protamine suspension)
- HUMALOG MIX50 (50% insulin lispro injection, 50% insulin lispro protamine suspension)

HUMALOG 200 units/mL prefilled pens are available in boxes containing 2 or 5 pens. The prefilled pen containing HUMALOG is not designed to be reused.

The HUMALOG contained in the HUMALOG 200 units/mL KwikPen should ONLY be injected with the KwikPen. Do not transfer insulin from your HUMALOG 200 units/mL KwikPen to a syringe or into a continuous subcutaneous insulin infusion pump. An insulin syringe or pump will not measure your dose correctly. A severe overdose can result, causing low blood sugar which may put your life in danger.

The HUMALOG contained in the HUMALOG 200 units/mL KwikPen must not be mixed with any other insulin.

For guidance on the use of the KwikPen (prefilled, disposable insulin injector), please refer to the separate Instructions for Use enclosed within the packaging.

DO NOT USE ANY OTHER INSULIN EXCEPT ON YOUR DOCTOR'S ADVICE AND DIRECTION.

Always keep an extra supply of HUMALOG i.e. a spare prefilled pen on hand. Always wear identification to indicate that you have diabetes so that appropriate treatment can be given if complications occur away from home.

When you receive your insulin from the pharmacy, always check to see that:

1. The name HUMALOG appears on the carton and prefilled pen label.
2. The carton and prefilled pen label is correct for your type of insulin.
3. The insulin strength is U-200.
4. The expiration date on the package will allow you to use the insulin before that date.

WARNINGS AND PRECAUTIONS

Serious Warnings and Precautions

- Hypoglycemia or low blood sugar is the most common adverse effect experienced by insulin users. Blood glucose monitoring is recommended for all patients with diabetes. Uncorrected hypoglycemic or hyperglycemic reactions can cause loss of consciousness, coma or even death. Information on how to recognize these symptoms is provided below.
- This Lilly human insulin analogue differs from other insulins because it has a unique structure, a very quick onset of action and a short duration of activity. HUMALOG should be given within 15 minutes before a meal or when necessary shortly after a meal instead (within 20 minutes of the start of the meal). The short duration of action of HUMALOG means that if you have Type 1 diabetes you also need to use a longer-acting insulin to give the best glucose control.
- HUMALOG should not be used if it is not water-clear and colourless or if it has formed a deposit of solid particles on the wall of the cartridge.
- Any change of insulin regimen should be made cautiously and only under medical supervision. Changes in purity, strength, brand (manufacturer), type (regular, NPH, etc), species (beef, pork, beef-pork, human), and/or method of manufacture (recombinant DNA versus animal-source insulin) may result in the need for a change in dosage.
- Patients taking HUMALOG may require a change in dosage from that used with other insulins. If an adjustment is needed, it may occur with the first dose or over a period of several weeks.
- HUMALOG 200 units/mL KwikPen is reserved for the treatment of patients with diabetes requiring daily doses of > 20 units of fast-acting insulin.

- HUMALOG 200 units/mL cannot be transferred from the HUMALOG 200 units/mL KwikPen to a syringe or insulin pump. An insulin syringe or pump will not measure the dose correctly. Overdose can result causing low blood sugar which may put your life in danger.
- HUMALOG 200 units/mL should not be mixed with any other insulin.
- The HUMALOG 200 units/mL KwikPen is designed to allow you to give more doses than other pens you may have used in the past. Dial your usual dose as instructed by your healthcare professional.

BEFORE you use HUMALOG talk to your doctor or pharmacist if:

- You have trouble with your kidneys or liver, your doctor may decide to alter your insulin dose.
- You drink alcohol (including wine and beer): watch for signs of hypoglycemia and never drink alcohol on an empty stomach.
- You exercise more than usual or if you want to change your usual diet. Exercise may lower your body's need for insulin during and for some time after the activity. Exercise may also speed up the effect of an insulin dose, especially if the exercise involves the area of injection site.
- You are ill. Illness, especially with nausea and vomiting, may cause your insulin requirements to change. Even if you are not eating, you will still require insulin. You and your doctor should establish a sick day plan for you to use in case of illness. When you are sick, test your blood/urine frequently.
- You are travelling across more than 2 time zones. You should consult your doctor concerning adjustments in your insulin schedule.
- You are pregnant. HUMALOG can be used in pregnancy if clinically indicated. Data on a large number of exposed pregnancies do not indicate any adverse effect of HUMALOG on pregnancy or on the health of the foetus/newborn. Good control of diabetes is especially important for you and your unborn baby. Pregnancy may make managing your diabetes more difficult. If you are planning to have a baby, are pregnant, or are nursing a baby, consult your doctor.
- When you use other medicines. Many medicines affect the way glucose works in your body and this may influence your insulin dose. Listed below are the most common medicines, which may affect your insulin treatment. Talk to your doctor or pharmacist if you take, or change any other medicines, even those not prescribed.

INTERACTIONS WITH THIS MEDICATION

Insulin requirements may be increased if you are taking other drugs with hyperglycemic activity, such as oral contraceptives (for example, birth control pills, injections and patches), corticosteroids, or thyroid replacement

therapy. Insulin requirements may be decreased in the presence of agents such as oral antidiabetic agents, salicylates (aspirin), sulfa antibiotics, certain antidepressants (monoamine oxidase inhibitors), beta-blockers, alcohol, ACE-inhibitors and angiotensin II receptor blockers. Always discuss any medications you are taking with your doctor.

The use of thiazolidinediones (such as rosiglitazone and pioglitazone), alone or in combination with other antidiabetic agents (including insulin), has been associated with heart failure and swelling of the lower extremities. Please contact your physician immediately if you develop symptoms of shortness of breath, fatigue, exercise intolerance, or swelling of the lower extremities while you are on these agents.

PROPER USE OF THIS MEDICATION

HUMALOG is a sterile solution. HUMALOG should be given by subcutaneous injection. The concentration of HUMALOG 200 units/mL in the prefilled pens is 200 units/mL (U-200).

When used as a meal-time insulin, HUMALOG should be given within 15 minutes before a meal, or when necessary shortly after a meal instead (within 20 minutes of the start of the meal).

HUMALOG is a clear and colourless liquid with a water-like appearance and consistency. Do not use if it appears cloudy, thickened, or slightly coloured or if solid particles are visible. Always check the appearance of your HUMALOG prefilled pen before using, and if you note anything unusual in its appearance or notice your insulin requirements changing markedly, consult your doctor.

Injection Procedure

Injecting the Dose:

1. Wash your hands.
2. Use an alcohol swab to wipe the exposed rubber surface on the metal cap end of the prefilled pen.
3. Inspect the HUMALOG in the cartridge contained in the prefilled pen. It should look clear and colourless. Do not use HUMALOG if it appears cloudy, thickened, or slightly coloured or if solid particles are visible.
4. Follow pen manufacturer's directions for attaching needle.
5. Hold the pen with needle pointing straight up. If there are large bubbles, tap the side of the pen until they float to the top. Remove the bubbles and the air in the needle by setting the pen to a 2-unit dose and depressing the plunger. Repeat this step if necessary until a drop of HUMALOG appears at the end of the needle.
6. To avoid tissue damage (skin thinning, skin thickening, or skin lumps), injection sites can be rotated so that the same site is not used more than approximately once a month.
7. Prepare the injection site as directed by your healthcare professional.
8. Insert the needle as instructed by your doctor.
9. To inject HUMALOG, follow the pen manufacturer's instructions.

10. Pull the needle out and apply gentle pressure over the injection site for several seconds. Do not rub the area.
11. Immediately after an injection, remove the needle from the pen. This will guard against contamination and prevent leakage, re-entry of air, and potential needle clogs. Dispose of the needle in a closable, puncture-resistant sharps container (like a biohazard container) or as directed by your healthcare professional. Do not reuse needle. **NEEDLES AND PENS MUST NOT BE SHARED.** To prevent the possible transmission of disease, never share a HUMALOG 200 units/mL pen between patients, even if the needle on the delivery device is changed.

The prefilled pen will not let you dial more than the number of units left in the pen. The cartridge contains an additional small amount of insulin that cannot be delivered. Do not transfer this to a syringe. Severe overdose can result.

Usual dose

Your doctor has told you which insulin to use, how much, and when and how often to inject it. Because each patient's case of diabetes is different, this schedule has been individualized for you.

Your usual HUMALOG dose may be affected by changes in your food, activity, or work schedule. Carefully follow your doctor's instructions to allow for these changes. Other things that may affect your HUMALOG dose are illness, pregnancy, medication, exercise and travel.

Overdose

Hypoglycemia (too little glucose in the blood) is one of the most frequent adverse events experienced by insulin users. It can be brought about by:

1. Missing or delaying meals
2. Taking too much insulin
3. Exercising or working more than usual
4. An infection or illness (especially with diarrhea or vomiting)
5. A change in the body's need for insulin
6. Diseases of the adrenal, pituitary, or thyroid gland, or progression of kidney or liver disease
7. Interactions with other drugs that lower blood glucose, such as oral hypoglycemics, salicylates, sulfa antibiotics, and certain antidepressants
8. Consumption of alcoholic beverages

Dietary Implications:

If a usual meal cannot be obtained at the appropriate time, then to avoid hypoglycemia, you should take the amount of carbohydrate prescribed for this meal in the form of orange juice, syrup, candy, or bread and milk, without changing your insulin dosage. If it becomes necessary to omit a meal on account of nausea and vomiting, you should test your blood sugar level and notify your doctor.

Mild to moderate hypoglycemia may be treated by eating foods or drinks that contain sugar. Patients should always carry a quick source of sugar, such as candy mints or glucose tablets. More severe hypoglycemia may require the assistance of another person. Patients who are unable to take sugar orally or who are unconscious should be treated with intravenous administration of glucose at a medical facility or should be given an injection of glucagon (either intramuscular or subcutaneous). The patient should be given oral carbohydrates as soon as consciousness is recovered.

In case of drug overdose, contact a healthcare practitioner, hospital emergency department or regional Poison Control Centre immediately, even if there are no symptoms.

SIDE EFFECTS AND WHAT TO DO ABOUT THEM

Hypoglycemia:

One of the most frequent adverse events experienced by insulin users is hypoglycemia (see PROPER USE OF THIS MEDICATION).

Diabetic Acidosis and Coma:

Diabetic acidosis may develop if your body has too little insulin (this is the opposite of insulin reaction, which is the result of too much insulin in the blood). Diabetic acidosis may be brought on if you omit your insulin or take less than the doctor has prescribed, eat significantly more than your diet calls for, or develop a fever or infection. With acidosis, urine tests show a large amount of sugar and acetone.

The first symptoms of diabetic acidosis usually come on gradually, over a period of hours or days, and include a drowsy feeling, flushed face, thirst, and loss of appetite. Heavy breathing and a rapid pulse are more severe symptoms.

If uncorrected, loss of consciousness, coma, or death can result. Therefore, it is important that you obtain medical assistance immediately.

Lipoatrophy, Lipohypertrophy, or Localized Cutaneous Amyloidosis:

Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the skin), lipohypertrophy (enlargement or thickening of tissue), or localized cutaneous amyloidosis (skin lumps). If you notice any of these conditions, consult your doctor. A change in your injection technique may help alleviate the problem.

Allergy to Insulin:

Patients occasionally experience redness, swelling, and itching at the site of injection of insulin. This condition, called local allergy, usually clears up in a few days to a few weeks. If you have local reactions, contact your doctor, who may recommend a change in the type or species of insulin.

Less common, but potentially more serious, is generalized allergy to insulin, which may cause rash over the whole body,

shortness of breath, wheezing, reduction in blood pressure, fast pulse, or sweating. Severe cases of generalized allergy may be life threatening. If you think you are having a generalized allergic reaction to insulin, notify a doctor immediately. Your doctor may recommend skin testing, that is, injecting small doses of other insulins into the skin, in order to select the best insulin for you to use. Patients who have had severe generalized allergic reactions to insulin should be skin tested with each new preparation to be used before treatment with that preparation is started.

This is not a complete list of side effects. For any unexpected effects while taking HUMALOG, contact your doctor or pharmacist.

HOW TO STORE IT

Prior to first use, HUMALOG 200 units/mL KwikPen prefilled pens should be stored in a refrigerator between 2° and 8°C. Do not freeze. Do not expose to excessive heat or sunlight. The HUMALOG 200 units/mL KwikPen that you are currently using should not be refrigerated but should be kept as cool as possible (below 30°C) and away from direct heat and light. Do not use HUMALOG if it has been frozen. Prefilled pens in use, or not refrigerated, should be discarded after 28 days, even if they still contain HUMALOG.

DO NOT USE THE HUMALOG 200 UNITS/ML KWIKPEN AFTER THE EXPIRATION DATE STAMPED ON THE LABEL.

Dispose of used needles in a puncture-resistant container or as directed by your healthcare professional.

Dispose of used pens as instructed by your healthcare professional and without the needle attached.

REPORTING SUSPECTED SIDE EFFECTS

You can report any suspected adverse reactions associated with the use of health products to the Canada Vigilance Program by one of the following 3 ways:

- Report online at www.healthcanada.gc.ca/medeffect
- Call toll-free at 1-866-234-2345
- Complete a Canada Vigilance Reporting Form and:
 - Fax toll-free to 1-866-678-6789, or
 - Mail to:
 - Canada Vigilance Program
 - Health Canada
 - Postal Locator 0701D
 - Ottawa, Ontario
 - K1A 0K9

Postage paid labels, Canada Vigilance Reporting Form and the adverse reaction reporting guidelines are available on the MedEffect™ Canada Web site at www.healthcanada.gc.ca/medeffect

NOTE: Should you require information related to the management of side effects, contact your health professional. The Canada Vigilance Program does not provide medical advice.

MORE INFORMATION

For more information, please contact your healthcare professionals or pharmacist first, or Eli Lilly Canada Inc. at:

1-888-545-5972 or visit the website at www.lilly.ca.

The information in this document is current as of the last revision date shown below. For the most current information please visit our website or contact us directly.

This leaflet was prepared by Eli Lilly Canada Inc.

HUMALOG, MIX25, MIX50 and KwikPen are registered trademarks owned by Eli Lilly and Company, its subsidiaries or affiliates.

You may need to read this package insert again. Please do not throw it away until you have finished your medicine.

Last revised: April 12, 2021

LOG200-0002-CA-PMI-2021MMDD