

Product Monograph
Including Patient Medication Information

Pr ARTISS

Fibrin Sealant (Human), Slow Set
Frozen Solutions for Thawing for Topical Application
4 IU/mL (Total Volumes: 2mL, 4mL, 10mL)

Haemostatic and Tissue Adhesive Agent

ATC code: B02BC30

Baxter Corporation
Mississauga, ON
Canada L5N 0C2

Date of Authorization:
2025-09-03

Control Number: 296800

Baxter, Artiss, Duplocath, Duploject, Duplospray, Easyspray, and Tisseel are trademarks of Baxter International Inc.

Recent Major Label Changes

4.4 Administration	2025-06
--------------------	---------

Recent Major Label Changes	2
Part 1: Healthcare Professional Information	4
1. Indications	4
1.1. Pediatrics.....	4
1.2. Geriatrics.....	4
2. Contraindications	4
3. Serious Warnings and Precautions Box	4
4. Dosage and Administration	5
4.2. Recommended Dose and Dosage Adjustment	5
4.4. Administration	5
5. Overdose	12
6. Dosage Forms, Strengths, Composition, and Packaging	12
7. Warnings and Precautions	14
General	14
Immune	16
Reproductive Health.....	17
7.1. Special Populations.....	17
7.1.1. Pregnancy.....	17
7.1.2. Breastfeeding.....	17
7.1.3. Pediatrics.....	17
7.1.4. Geriatrics.....	17
8. Adverse Reactions	18
8.1. Adverse Reaction Overview	18
8.2. Clinical Trial Adverse Reactions	18
8.2.1. Clinical Trial Adverse Reactions – Pediatrics.....	20
8.3. Less Common Clinical Trial Adverse Reactions.....	20
8.5. Post-Market Adverse Reactions.....	20
9. Drug Interactions	21

9.2.	Drug Interactions Overview	21
9.3.	Drug-Behaviour Interactions.....	21
9.4.	Drug-Drug Interactions	21
9.5.	Drug-Food Interactions.....	21
9.6.	Drug-Herb Interactions	21
9.7.	Drug-Laboratory Test Interactions.....	21
10.	Clinical Pharmacology.....	21
10.1.	Mechanism of Action	21
10.2.	Pharmacodynamics.....	22
10.3.	Pharmacokinetics.....	22
10.4.	Immunogenicity	22
11.	Storage, Stability, and Disposal	22
Part 2: Scientific Information		24
13.	Pharmaceutical Information	24
14.	Clinical Trials	28
14.1.	Clinical Trials by Indication	29
14.2.	Comparative Bioavailability Studies	35
15.	Microbiology	36
16.	Non-Clinical Toxicology	36
Patient Medication Information		38

Part 1: Healthcare Professional Information

1. Indications

ARTISS (Fibrin Sealant (Human), Slow Set) is indicated for:

- the fixation (gluing) of autologous skin grafts and tissue flaps.
- as an adjunct to haemostasis on subcutaneous tissue surfaces to treat burns in adult and pediatric patients.
- as an adjunct to adhere tissue flaps during facial rhytidectomy surgery (face-lift).

1.1. Pediatrics

Pediatrics (1.1 – 16 years of age) or (< 16 years of age):

Efficacy and safety in the use of ARTISS (Fibrin Sealant (Human), Slow Set) has been evaluated in a clinical trial involving a group of pediatric patients and was not found to be different from an adult population.

1.2. Geriatrics

Geriatrics (> 65 years of age):

Efficacy and safety in use of ARTISS (Fibrin Sealant (Human), Slow Set) has been evaluated in a clinical trial involving a small number of geriatric patients. No overall differences in safety or effectiveness were observed between these subjects and younger subjects.

2. Contraindications

- ARTISS (Fibrin Sealant (Human), Slow Set) is contraindicated in patients who are hypersensitive to this drug or to any ingredient in the formulation including any non-medicinal ingredient or component of the container. For a complete listing, [see 6 DOSAGE FORMS, STRENGTHS, COMPOSITION AND PACKAGING](#).
- ARTISS is contraindicated in individuals with a known hypersensitivity to Aprotinin.
- ARTISS is contraindicated for intravascular application and should not be injected directly into a blood vessel. Intravascular application may result in life threatening thromboembolic events.
- ARTISS alone should not be used for the treatment of massive brisk arterial or venous bleeding as it is not effective in this situation.

3. Serious Warnings and Precautions Box

- Life threatening thromboembolic events have occurred when ARTISS (Fibrin Sealant (Human), Slow Set) was inadvertently administered intravascularly (see [7 WARNINGS AND PRECAUTIONS, Vascular Disorders](#)).

- Fatal air or gas embolism has occurred with application of ARTISS using pressurized air or gas (see [4 DOSAGE AND ADMINISTRATION](#) and [7 WARNINGS AND PRECAUTIONS, Vascular Disorders](#))
- Severe hypersensitivity and anaphylactic reactions have been reported with ARTISS. Adequate medical treatment and provisions should be available for immediate use in the event of an anaphylactic reaction (see [7 WARNINGS AND PRECAUTIONS, Immune.](#))
- ARTISS is made from pooled human plasma which may contain infectious agents, such as viruses, that can cause disease (see [7 WARNINGS AND PRECAUTIONS, General](#))

4. Dosage and Administration

4.2. Recommended Dose and Dosage Adjustment

Application of the product must be individualized to the patient by the treating physician. In clinical trials, the individual dosages have typically ranged from 0.2-12 mL. For some procedures (e.g., the sealing of large, burned surfaces), larger volumes may be required.

The initial amount of the product to be applied at a chosen anatomic site or target surface area should be sufficient to entirely cover the intended application area. The application can be repeated, if necessary. However, avoid re-application of ARTISS (Fibrin Sealant (Human), Slow Set) to a pre-existing polymerized ARTISS layer as ARTISS may not adhere firmly to a polymerized layer.

The amount of ARTISS to be applied depends on the size of the surface to be covered. The approximate surface areas covered by each package size of ARTISS are listed in the following table:

Table 1: Approximate Surface Areas Covered by Each Package Size of ARTISS

Area to be sealed (cannula, catheter)	Area to be sealed using compressed gas (spray application)	Required package size of ARTISS
8 cm ²	25-100 cm ²	2 mL
16 cm ²	50-200 cm ²	4 mL
40 cm ²	125-500 cm ²	10 L

4.4. Administration

For topical use only – do not inject.

ARTISS is available as frozen solutions for thawing.

ARTISS consists of a pre-filled double-chamber syringe (PRIMA syringe) containing Sealer

Protein-Aprotinin Solution and Thrombin-Calcium Chloride Solution. ARTISS is available in 2, 4 and 10 mL pack sizes.

Various methods can be used to simultaneously apply the two components of ARTISS:

- using application cannula contained in DUPLOJECT COMBI
- using TISSEEL / ARTISS Spray Set and EASYSPRAY Pressure Regulator
- using DUPLOCATH Application Catheters or other accessories provided by Baxter

Preparation of ARTISS

- Do not use ARTISS unless it is completely thawed and warmed (liquid consistency).
- ARTISS must not be exposed to temperatures above 37°C and must not be microwaved.
- The protective syringe cap should not be removed until thawing is complete, and application tip is ready to be attached.

ARTISS may be thawed and warmed under controlled conditions using one of the two following options:

Quick Thawing/Warming Methods

An Overview of the quick thawing/warming methods is provided in Table 2

Table 2: Quick Thawing /Warming Methods at 33°C – 37°C

Pack Size	Minimum Thawing/Warming Times		
	Sterile Water Bath (Pouches Removed)	Non-Sterile Water Bath (In Pouches)	Incubator (In Pouches)
2 mL	5 min	15 min	40 min
4 mL	5 min	20 min	50 min
10 mL	10 min	35 min	90 min

Sterile Water Bath (Recommended Method)

- Transfer the pre-filled syringe packed in the inner pouch into the sterile area.
- Remove the pre-filled syringe from the inner pouch and place the syringe directly into the sterile water heated to 33°C - 37°C ensuring the syringe is completely immersed in the water (See Table 2 for minimum thawing/warming times).
- To monitor the specified temperature range, control the water temperature using a thermometer and change the water as necessary.

Non-Sterile Water Bath

- Place the pre-filled syringe packed in both pouches, in a water bath heated to 33°C - 37°C outside the sterile area, ensuring the pouches remain immersed in the water (See Table 2 for minimum thawing/warming times).

- Remove the pouches from the water bath after thawing and warming.
- Dry the outer pouch and transfer the pre-filled syringe in the inner pouch, onto the sterile area.

Incubator

- Place the pre-filled syringe, packed in both pouches, in an incubator outside the sterile area (See Table 2 for minimum thawing/warming times).
- After thawing/warming in the incubator, remove the outer pouch and transfer the pre-filled syringe, inside the inner pouch, into the sterile area.

Thawing at Room Temperature (not above +25°C) followed by Warming in Incubator

- Thaw the pre-filled syringe, packed in both pouches, at room temperature outside the sterile area (See Table 3 for minimum thawing times).
- Warm the pre-filled syringe, packed in both pouches, in an incubator at 33°C-37°C outside the sterile area (See Table 3 for minimum thawing/warming times).
- After thawing/warming in the incubator, remove the outer pouch and transfer the pre-filled syringe, inside the inner pouch, into the sterile area.

Table 3: Thawing at Room Temperature and warming in Incubator

Pack Size	Minimum Thawing/Warming Times	
	Thawing at Room Temperature (Not above +25°C)	Warming in Incubator (33°C-37°C)
2 mL	80 min	11min
4 mL	90 min	13 min
10 mL	160 min	25 min

Stability after Thawing

After quick thawing and warning: Once the package is opened or the product is warmed to 33°C to 37°C, it must be used within 12 hours.

Product thawed at room temperature: Unopened pouches of ARTISS, may be stored for up to 7 days at room temperature (15°C to 25°C) after removal from the freezer.

After thawing, the product must not be refrigerated or, refrozen.

Method of Application

Application Considerations

See [7 WARNINGS AND PRECAUTIONS, General](#) and [Application Precautions](#).

The use of ARTISS is restricted to experienced surgeons who have been trained in the use of ARTISS.

The setting rate depends on the concentration of human Thrombin contained in the Thrombin-

Calcium Chloride solution used. The ARTISS Thrombin component is provided in a 4 IU/mL concentration. Time to clot formation/ polymerization may take up to one minute to set with a Thrombin concentration of 4 IU/mL. Use of ARTISS is appropriate for surgical procedures where sufficient time for manipulation of tissues and approximation of the wound areas is demanded to glue tissues (e.g., skin grafts, tissue flaps, etc.). A 500 IU/mL Thrombin concentration is also available and marketed as TISSEEL 500 IU, Fast Set.

The sealer protein and the thrombin solutions should be clear or slightly opalescent. Do not use solutions that are cloudy, discolored, have deposits or other changes in their appearance.

Choice of Application Method/Device

- The cannulas included with DUPLOJECT COMBI System may be used for small wounds or for edges of a skin graft that did not adhere to the wound bed.
- In operation sites where access is difficult, ARTISS can be applied using DUPLOCATH Application Catheters.
- TISSEEL / ARTISS Spray Set is particularly suitable for spraying of larger areas.

Caution must be used when applying fibrin sealant using pressurized air or gas. Life-threatening/fatal air or gas embolism has occurred with the use of spray devices employing a pressure regulator to administer fibrin sealants. This event appears to be related to the use of the spray device at higher than recommended pressures and in close proximity to the tissue surface. The risk appears to be higher when fibrin sealants are sprayed with air, as compared to CO₂ and therefore cannot be excluded when ARTISS is used during open wound surgery.

General Application Instructions

- Before the application of ARTISS, ensure that all parts of the body outside the desired application area are sufficiently covered to prevent tissue adhesion at undesired sites.
- Prior to applying ARTISS the surface area of the wound needs to be dried by standard techniques (e.g., intermittent application of compresses, swabs, use of suction). Do not use pressurized air or gas for drying the site.
- Apply the mixed sealer protein - thrombin solution on to the recipient surface or on to the surfaces of the parts to be glued by slowly pressing on the back of the common plunger.
- In surgical procedures that require the use of minimal volumes of fibrin sealant, it is recommended to expel and discard the first few drops of product.
- After ARTISS has been applied, allow at least 3 minutes to achieve sufficient polymerization.
- To prevent ARTISS from adhering to gloves and instruments, wet these with saline before contact with Sealant.
- Ensure that the two components are quickly and thoroughly mixed, which is essential for ARTISS to gain the optimum strength. Once turbid, ARTISS can no longer be manipulated.
- Immediately before application, expel and discard the first several drops from the application cannula to ensure use of adequately mixed product. Separate, sequential

application of the two components must be avoided.

- Note: If application is interrupted, clogging will occur quickly in the cannula. In this case, replace the application cannula with a new one only immediately before application is resumed. If the openings of the joining piece are clogged, use the spare joining piece provided in the package. Application is also possible with other accessories supplied by BAXTER that are particularly suited for, e.g. application to large or difficult-to-access areas. When using these application devices, strictly follow the Instructions for Use of the devices.
- The skin graft should be attached to the wound bed immediately after ARTISS has been applied. The surgeon has up to 60 seconds to manipulate and position the graft prior to polymerization.
- If ARTISS does not fully adhere to tissue and bleeding continues, remove ARTISS clot and repeat application.
- After the flap or graft has been positioned, hold in the desired position by gentle compression for at least 3 minutes to ensure ARTISS sets properly, and the flap or graft adheres firmly to the underlying tissue.
- Solidified Sealant reaches its ultimate strength after about two hours (70% after about ten minutes).

Application Instructions by Device

a) Simultaneous Application using application cannula contained in DUPLOJECT COMBI

For application, connect the double chamber ready-to-use syringe with the sealer protein solution and the thrombin solution to a joining piece and an application cannula – both are provided in the set with the application devices. The common plunger of the double chamber ready-to-use syringe ensures that equal volumes of the two sealant components are fed through the joining piece into the application cannula where they are blended and then applied.

Operating Instructions



- To facilitate removal of the tip cap from the syringe, rock the tip cap by moving it backward and forward, then pull the protective cap off the syringe.
- Expel all air from the syringe prior to attaching any application device.
- Align the joining piece and tether to the side of the syringe with the tether strap hole.
- Connect the nozzles of the double chamber ready-to-use syringe to the joining piece, ensuring that they are firmly attached.
 - Secure the joining piece by fastening the tether strap to the double chamber ready-to-use syringe.
 - If the tether strap tears, use the spare joining piece provided in the kit.
 - If a spare joining piece is not available, the system can still be used if care is taken to ensure that the connection is secure and leak-proof.
 - Do NOT expel the air remaining inside the joining piece.
- Attach an application cannula on to the joining piece.
 - Do NOT expel the air remaining inside the joining piece and inside the application cannula until you start the actual application because this may clog the application cannula.

b) Simultaneous Application Using Spray Set and EASYSPRAY:

Caution must be used when applying fibrin sealant using pressurized air or gas.

- Any application of air or pressurized gas is associated with a potential risk of air or gas embolism, tissue rupture, or gas entrapment with compression, which may be life-threatening.
- ARTISS must be sprayed only onto application sites that are visible.
- ARTISS must not be applied intravascularly. (See [7 WARNINGS AND PRECAUTIONS](#))

Note: For operation instructions please refer to the Instructions for Use provided together with TISSEEL / ARTISS Spray Set and EASYSPRAY Pressure Regulator.



The TISSEEL / ARTISS Spray Set is particularly suitable for spraying of larger areas, e.g., to control oozing of parenchymatous organs or to adhere skin grafts. The two components are sprayed simultaneously using sterile propellant gas via EASYSpray Pressure Regulator, and the volume of the Solutions ejected is controlled with the PRIMA syringe plunger.

When applying ARTISS using EASYSpray Pressure Regulator and TISSEEL / ARTISS Spray Set, be sure to use a pressure and a distance from tissue within the ranges recommended by the manufacturer as follows:

Table 4: Recommended pressure, distance and devices for spray application of ARTISS

Surgery	Spray set/Applicator tips to use	Pressure regulator to be used	Gas	Recommended distance from target tissue	Recommended spray pressure
Open wound surgery of subcutaneous tissue	Artiss Spray Set	EasySpray	Medical grade CO ₂ *, Compressed Air or Nitrogen	10 – 15 cm	1.5-2.0 bar (21.8-29.0 psi)
	Artiss Spray Set 10 pack	EasySpray			

* Medical grade CO₂ is the preferred gas for application, however compressed air or nitrogen are acceptable gases for administration of ARTISS in open surgery.

Equivalent spray devices, intended for specific use with ARTISS, may also be used. When using other spray devices, follow the instructions for use that are provided with the device.

When using accessory tips with this product, the instructions for use of the tips should be followed.

c) Simultaneous Application Using DUPLOCATH Application Catheters or other accessories provided by Baxter:

In operation sites where access is difficult, ARTISS can be applied using DUPLOCATH Application Catheters or equivalent spray devices, intended for specific use with ARTISS, may also be used.

Note: When using other spray devices, please follow the Instructions for Use provided together with DUPLOCATH Application Catheter 25 or the instructions for use that are provided with the device.

In case of using other accessories provided by Baxter, please refer to the operating instructions contained in the Instructions for Use for the particular accessory.

When spraying ARTISS, changes in blood pressure, pulse, oxygen saturation and end tidal CO₂ should be monitored because of the possibility of occurrence of air or gas embolism.

5. Overdose

As the product is actively used by the surgeon, overdose is very unlikely to occur. ARTISS (Fibrin Sealant (Human), Slow Set) is only to be used by a physician in a hospital setting.

Excessive thickness of the fibrin layer may negatively interfere with the product's efficacy and the wound healing process (see 4 Dosage and Administration and 7 Warnings and Precautions)

For the most recent information in the management of a suspected drug overdose, contact your regional poison control centre or Health Canada's toll-free number, 1-844 POISON-X (1-844-764-7669).

6. Dosage Forms, Strengths, Composition, and Packaging

To help ensure the traceability of biologic products, health professionals should recognise the importance of recording both the brand name and the non-proprietary (active ingredient) name as well as other product-specific identifiers such as the Drug Identification Number (DIN) and the batch/lot number of the product supplied. As with other aprotinin-containing products, documentation in the patient's records should indicate that ARTISS contains aprotinin.

Dosage Forms and Packaging

ARTISS (Fibrin Sealant (Human), Slow Set) is available as frozen solutions for thawing.

Table 5: Dosage Forms, Strengths, Composition and Packaging

Route of Administration	Dosage Form / Strength / Composition	Volume (Total)	Non-medicinal Ingredients
Topical	4 IU/mL Frozen Solutions for Thawing	2 mL 4 mL 10 mL	1.0 mL/ 2.0 mL/ 5.0 mL of sterile frozen ARTISS Sealer Protein (Human)-Aprotinin Solution 1.0 mL/ 2.0 mL/ 5.0 mL of sterile frozen Thrombin (Human) – Calcium Chloride Solution

ARTISS also contains DUPLOJECT COMBI, the sterile accessory device set consisting of 2 joining pieces and 4 application cannulas.

The rubber stoppers are not made with natural rubber latex.

See the following Accessories Section for more accessories for use with ARTISS.

Composition

ARTISS consists of a double-chamber syringe containing Sealer Protein-Aprotinin (synthetic) Solution (syringe body 1) and Thrombin-Calcium Chloride Solution (syringe body 2).

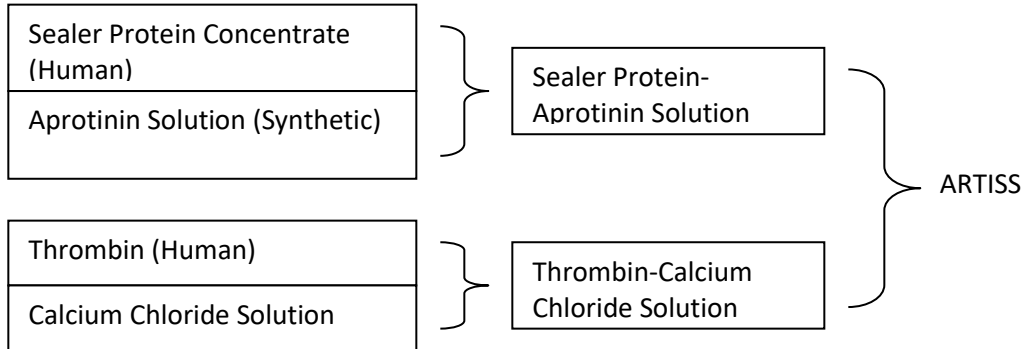


Table 6: Composition of ARTISS Solutions in Syringe Body 1 and Syringe Body 2

	Component	Amount
1	Sealer Protein (Human)-Aprotinin Solution, sterile, contains:	
	- Total protein	96-125 mg/mL
	- Factor XIII	0.6-10 U/mL**
	- Fibrinogen (Clottable Protein)	72-110 mg/mL
	- Plasmafibrinectin (CIG)*	2-9 mg/mL
	- Plasminogen*	40 – 120 µg/mL
	- Aprotinin (synthetic) Solution, sterile	3,000 KIU/mL***
2	Thrombin (Human)-Calcium Chloride Solution, sterile, contains:	
	Thrombin (Human)	2.5 - 6.5 IU/mL****
	Calcium Chloride Solution, sterile	36 - 44 µmol/mL

* Development data, not tested at the Final Product level

** One unit corresponds to the amount of Factor XIII contained in 1 mL of fresh normal plasma.

*** 30 Kallidinogenase Inactivator Units (KIU) correspond to 1 FIP-Unit².

**** One International Unit (IU) of Thrombin is defined as the activity contained in 0.0853 mg of the First International Standard of Human Thrombin³.

Nonmedicinal ingredients in the Sealer Protein-Aprotinin solution are human albumin, niacinamide and water for injection (WFI). Nonmedicinal ingredients in the Thrombin-Calcium Chloride solution are human albumin, sodium chloride and water for injection (WFI). Sodium Hydroxide and Hydrochloric Acid are used to adjust the pH in both solutions.

Accessories

The following are some accessories for use with ARTISS. A complete list of accessories can be obtained from a Baxter representative. When using these devices, strictly follow the Instructions for Use of the devices.

Table 7: Accessories Available for Use with ARTISS

EASYSpray Pressure Regulator	Propellant gas control unit, manometer, reducing valve, and pressure tube.
TISSEEL / ARTISS Spray Set (sterile, disposable)	Disposable set consisting of sterile filter with pressure line, sensing line and a spray head.
DUPLOCATH 25 Application Catheter	Length: approximately 25 cm (10") Diameter: approximately 5 french (approx. 0.17 cm) Radiopaque. Sterile. Disposable.

7. Warnings and Precautions

Please see **Error! Reference source not found. Error! Reference source not found..**

This product is prepared from large pools of human plasma. Thus, there is a possibility it may contain causative agents of viral or other undetermined diseases.

General

ARTISS (Fibrin Sealant (Human), Slow Set) is made from human plasma. Products made from human plasma may contain infectious agents, such as viruses, that can cause disease. This also applies to unknown or emerging viruses and other pathogens. The risk that such products will transmit an infectious agent has been reduced by screening plasma and by inactivating and removing certain viruses. All plasma units used for manufacture are ALT tested and non-reactive in tests for Hbs-antigen and antibodies to HCV, HIV-1 and HIV-2. Before further processing all individual plasma donations are subjected to an inventory hold for a possible look-back of plasma donations suspected of infection. All plasma units are tested by HIQ-PCR = Hyland Immuno Quality Assured Polymerase Chain Reaction.

Despite these measures, plasma products may still carry a risk of transmitting infectious agents, e.g., unknown viruses, and theoretically, the Creutzfeldt-Jakob disease (CJD) agent. There is also the possibility that unknown infectious agents may be present in such products. Individuals who receive infusions of blood or plasma products may develop signs and/or symptoms of some viral infections.

The measures taken are considered effective for inactivation/removal of enveloped viruses such as HIV, HBV, and HCV, and for the non-enveloped virus HAV.

Some viruses, such as parvovirus B19, are particularly difficult to remove or inactivate at this time. Parvovirus B19 most seriously affects pregnant women (fetal infection) and individuals with immunodeficiency or increased red blood cell turnover.

This product must not be used in animals.

Application Precautions

(See also 4 DOSAGE AND ADMINISTRATION-Application Considerations)

Solutions containing alcohol, iodine or heavy metals may interfere with the product's performance due to denaturation of proteins or other mechanisms. If any of these substances have been used to clean the wound area, the area must be thoroughly rinsed before application of ARTISS.

ARTISS is not indicated for haemostasis in situations where a fast clotting of a sealant is required.

Intravascular application of ARTISS must be avoided as it can lead to intravascular coagulation, may result in life-threatening thromboembolic events and might increase the likelihood and severity of acute hypersensitivity reactions in susceptible patients.

Injection into the nasal mucosa must be avoided, as severe allergic-anaphylactoid reactions have been seen and thromboembolic events may occur.

Only a thin layer of ARTISS should be applied to avoid the formation of excess granulation tissue and to ensure gradual absorption of the solidified fibrin sealant. Excessive thickness of the fibrin layer may negatively interfere with the product's efficacy and the wound healing process (see [4 DOSAGE AND ADMINISTRATION - Administration](#)).

Spray Application:

ARTISS spray application should only be used if it is possible to accurately judge the spray distance.

The user is cautioned against the spray application of ARTISS with devices produced by other manufacturers. The EASYSPRAY Pressure Regulator control device and the TISSEEL / ARTISS Spray Set may be obtained from Baxter. Only use application devices licensed for the administration of ARTISS.

ARTISS must not be used with the EASYSPRAY Pressure Regulator and TISSEEL/ ARTISS Spray Set system in enclosed body areas.

When spraying ARTISS, changes in blood pressure, pulse, oxygen saturation and end tidal CO₂, should be monitored because of the possibility of occurrence of air or gas embolism.

The risk of gas embolism can increase when the tissue surface gas pressure exceeds the peripheral venous pressure. Respecting the recommended distance and pressure limit prevents exceeding that threshold and includes a safety margin. To reduce the risk of a potentially life-threatening gas embolism when applying ARTISS using the EASYSPRAY Pressure

Regulator and TISSEEL / ARTISS Spray Set, be sure to use the pressure within the pressure range recommended by the spray device manufacturer. Do not spray at a pressure above 2 bar or at a distance closer than 10 cm from the surface of the tissue.

Easy Spray is designed with safety features to limit gas pressure within safe pressure range:

- Pressure Control Knob limits the user to selecting a gas pressure between 0.5 and 2.0 bar
- The Safety Valve cuts off gas flow when the pressure reaches 2.3 ± 0.2 bar
- If the pressure regulator is deficient, a piezo valve shuts the circuit to prevent delivering gas with overpressure.
- Settings on 100% of the devices are verified during release of the product
- The pressure regulator component is compliant with ISO 10524-4 standard, which sets requirements on accuracy as well as safety for low pressure regulators.
- Labeling on the device states the minimal spray distance.
- The Pressure Gauge shows safe pressure range in green with red indicating pressure is too high

Immune

Hypersensitivity or allergic/anaphylactoid reactions may occur with the use of ARTISS. Cases have been reported in post-marketing experience with fibrin sealant (8.5 Post-Market Adverse Reactions). In specific cases, these reactions have progressed to become life-threatening. Such reactions are more likely if ARTISS is applied repeatedly over time or in the same setting, or if systemic aprotinin has been administered previously; however, these reactions may also occur in patients receiving ARTISS for the first time. Even if the first treatment was well tolerated, a subsequent administration of ARTISS or systemic aprotinin may not exclude the occurrence of an allergic reaction. Symptoms associated with allergic anaphylactic reactions include flush, urticaria, pruritus, nausea, drop in blood pressure, tachycardia or bradycardia, dyspnea, severe hypotension and anaphylactic shock.

Aprotinin, a monomeric polypeptide, is included in ARTISS for its antifibrinolytic properties, and is known to be associated with anaphylactic reactions. Even in the case of strict local application of aprotinin, there is a risk of anaphylactic reactions to aprotinin, particularly in the case of previous exposure.

In the event of anaphylactic/anaphylactoid or allergic-type hypersensitivity reactions, discontinue administration of ARTISS. If possible, remove any applied, polymerized product from the surgical site. Allergic and anaphylactic reactions should be managed according to current medical guidelines. Mild reactions can be managed with antihistamines. Severe hypotensive reactions require immediate resuscitative intervention. Adequate medical treatment and provisions should be available for immediate use in the event of an anaphylactic reaction.

Reproductive Health

Animal reproduction studies have not been conducted with ARTISS. It is not known whether ARTISS can affect reproductive capacity.

Vascular Disorders

Air or Gas Embolism

Life-threatening/fatal air or gas embolism has occurred with the use of spray devices employing a pressure regulator to administer fibrin sealants. This event appears to be related to the use of the spray device at higher than recommended pressures and with the applicator tip in close proximity to the tissue surface. The risk appears to be higher when fibrin sealants are sprayed with air, as compared to CO₂ and therefore cannot be excluded when ARTISS is used during open wound surgery. Caution must be used when applying fibrin sealant using pressurized air or gas (see [4 DOSAGE AND ADMINISTRATION](#), [6 DOSAGE FORMS, STRENGTHS, COMPOSITION AND PACKAGING](#), [7 WARNINGS AND PRECAUTIONS – Application Precautions/Spray Application](#)).

Thromboembolic Events

Inadvertent intravascular application of sealants have led to thromboembolic events. Intravascular application must be avoided.

7.1. Special Populations

7.1.1. Pregnancy

The safety of fibrin sealants/haemostatics for use in human pregnancy, and during labor and delivery has not been studied.

Animal reproduction studies have also not been conducted with ARTISS. Health professionals should balance the potential risks and only prescribe ARTISS if clearly needed.

See 7 WARNINGS AND PRECAUTIONS for information on Parvovirus B19 infection.

7.1.2. Breastfeeding

It is unknown if ARTISS is excreted in human milk. Precaution should be exercised because many drugs can be excreted in human milk. Health professionals should balance the potential risks and only prescribe ARTISS if clearly needed.

7.1.3. Pediatrics

The required dose of the fibrin sealant depends on the size of the surface to be covered, and the application device used. No dosing adjustment or additional precautions are required.

7.1.4. Geriatrics

No dosing adjustment or additional precautions are required.

8. Adverse Reactions

8.1. Adverse Reaction Overview

The most common adverse reactions reported in clinical trials for ARTISS (Fibrin Sealant (Human), Slow Set) include skin graft failure (25.4%) and pruritis (20.3%) (See [Section 8.2 Clinical Trial Adverse Reactions](#)).

During post marketing surveillance rare reports of life-threatening thromboembolic events have been reported following the inadvertent intravascular administration of ARTISS.

Allergic and/or anaphylactic reactions may occur in patients with a history of hypersensitivity to Aprotinin. Such reactions may be seen in the event of repeated administration, even if the first application was well tolerated. However, allergic and/or anaphylactic reactions may also occur in patients receiving ARTISS for the first time. No adverse events of this type were reported during clinical trials for ARTISS.

8.2. Clinical Trial Adverse Reactions

Note: For a discussion of the product preparations used in the clinical trials please refer to [14 CLINICAL TRIALS](#).

Clinical trials are conducted under very specific conditions. The adverse reaction rates observed in the clinical trials, therefore, may not reflect the rates observed in practice and should not be compared to the rates in the clinical trials of another drug. Adverse reaction information from clinical trials may be useful for identifying and approximating rates of adverse drug reactions in real-world use.

Split Thickness Sheet Skin Grafts in Treatment of Burn Wounds

The following Adverse Reactions have been reported from a clinical trial where ARTISS (FS VH S/D 4 s-apr) was used to affix split thickness sheet skin grafts to excised burn wounds (see [14 CLINICAL TRIALS, Trial 550201](#)). All 138 subjects received two treatments (ARTISS and control) at separate sites. On the test site, ARTISS was used to secure the graft to the burn wound, and for the control site, staples (considered standard of care) were used to secure the graft to the burn wound. None of the events were classified as serious.

Table 8: Adverse Events in Study 550201 Occurring at ARTISS and Stapled Sites in $\geq 1.0\%$ of Subjects (N=138)

MedDRA System Organ Class/Preferred Term	ARTISS N=138 (%)	Stapled Site N=138 (%)
Infections and infestations:		
• Infections	6 (4.3)	7 (5.1)
Injury, poisoning, and procedural complications:		

• Skin graft failure	35 (25.4)	32 (23.2)
• Graft complication	2 (1.4)	14 (10.1)
Skin and subcutaneous tissue disorders:		
• Pruritus	28 (20.3)	29 (21.0)
• Dermal Cyst	2 (1.4)	3 (2.2)
• Excessive granulation tissue	2 (1.4)	1 (0.7)

There was no difference in the probability of occurrence of Serious Adverse Events (SAEs) between ARTISS test sites (4.3%; n= 6) and stapled test sites (3.6%; n= 5).

Facial Rhytidectomy

The following Adverse Reactions have been reported from clinical trials where ARTISS was used for adherence of skin flaps in facial rhytidectomy surgeries (see Part [II 14 CLINICAL TRIALS trial numbers 550703 and 550901](#)). Both studies had a split-face design: on the control side of the face, closure of the flap was achieved with staples and suturing (considered standard of care); on the other side of the face, closure of the flap was achieved with ARTISS as an adjunct to staples and suturing. Adverse events that occurred on the face at an overall frequency greater than or equal to 1% are shown in the table below.

Table 9: Adverse Events in Study 550703 and 550901 Occurring at ARTISS and/or Stapled Sites in ≥1.0% of Subjects (N=120) in Facial Rhytidectomy

MedDRA System Organ Class/Preferred Term	ARTISS Site employed ARTISS as an adjunct to staples and suturing N=120 (%)	“Stapled Site” refers to the control site where both staples and sutures were used N=120 (%)
Injury, poisoning and procedural complications		
• Seroma	4 (3.3)	6 (5.0)
General disorders and administration site conditions		
• Oedema	3 (2.5)	4 (3.3)
Injury, poisoning and procedural complications		
• Post procedural haematoma	1 (0.8)	a) 9.2)

* Percent is based on total number of subjects in safety analysis set: 120.

Three subjects experienced serious adverse events. Two were local: wound abscess on the ARTISS treated side of the face that was recognized on postoperative day 14 and treated by operative incision and drainage; and a case of basal cell carcinoma on the control side of the face. A third subject experienced dehydration on the second postoperative day.

8.2.1. Clinical Trial Adverse Reactions – Pediatrics

Study 550201 included 40 pediatric subjects ranging in age from 1-18 (see [14 CLINICAL TRIALS](#)). The adverse reaction rates for pediatric subjects were consistent with the adult population. Although limitations apply due to the number of pediatric patients included in the clinical trial, no additional safety issues were noted in children.

8.3. Less Common Clinical Trial Adverse Reactions

The less common adverse events (that occurred in <1.0% of study participants who received ARTISS, classified by System Organ Class and in alphabetical order include:

- General disorders and administration site conditions: Oedema peripheral
- Injury, poisoning and procedural complications: Surgical wound with bacterial or fungus that can cause infection; Excoriation; Wound dehiscence
- Musculoskeletal and connective tissue disorders: Joint contracture
- Skin and subcutaneous tissue disorders: Skin maceration
- Vascular Disorders: Haematoma

8.5. Post-Market Adverse Reactions

The following adverse reactions have been identified during post-approval use of ARTISS. Because these reactions are reported voluntarily and the population is of uncertain size, it is not always possible to reliably estimate the frequency of these reactions.

Hypersensitivity Reactions:

Hypersensitivity reactions have been reported. Manifestations of hypersensitivity have included: application site irritation, chest discomfort, chills, headache, lethargy, restlessness, and vomiting. Severe hypersensitivity and anaphylactic reactions have also been reported in postmarket use.

Vascular disorders:

Air embolism*

- * as with other fibrin sealants, life-threatening/fatal air or gas embolism has occurred when using devices with pressurized air or gas; this event appears to be related to an inappropriate use of the spray device (e.g., at higher than recommended pressure and in close proximity to the tissue surface)

Thromboembolic events:

There have been rare reports of fatalities following the misadministration of topical thrombin. Life-threatening thromboembolic events have also been reported following inadvertent intravascular application of fibrin sealants.

9. Drug Interactions

9.2. Drug Interactions Overview

Drug Interactions are not known. No formal interaction studies have been performed. ARTISS (Fibrin Sealant (Human), Slow Set) can be applied in fully heparinized patients (e.g., extracorporeal circulation).

9.3. Drug-Behaviour Interactions

The interaction of ARTISS with individual behavioural risks has not been studied.

9.4. Drug-Drug Interactions

Interactions with other drugs have not been established.

Solutions containing alcohol, iodine or heavy metals may interfere with the product's performance due to denaturation of proteins or other mechanisms. If any of these substances have been used to clean the wound area, the area must be thoroughly rinsed before application of ARTISS.

Oxidized cellulose-containing preparations may reduce the efficacy of ARTISS and should not be used as carrier materials.

ARTISS must not be mixed with other medicinal products.

9.5. Drug-Food Interactions

Interactions with food have not been established.

9.6. Drug-Herb Interactions

Interactions with herbal products have not been established.

9.7. Drug-Laboratory Test Interactions

Interactions with laboratory tests have not been established.

10. Clinical Pharmacology

10.1. Mechanism of Action

The action of ARTISS (Fibrin Sealant (Human), Slow Set) simulates key features of the physiological process of wound closure. A highly concentrated fibrinogen Aprotinin solution, which among other ingredients contains Factor XIII co-fractionated from the plasma, and a

solution of thrombin and calcium chloride are applied to the wound area, where the mixture coagulates. The presence of Factor XIII causes the fibrin to crosslink, which gives the coagulum additional resilience. Aprotinin prevents premature degradation of the clot. As a biologic material, Fibrin Sealant becomes completely absorbed at a rate which depends both on the fibrinolytic activity of the surrounding tissue and the quantity of Fibrinolysis Inhibitor added. During wound healing the Sealant clot is gradually replaced by ingrowing tissue.

Spray application of ARTISS over the wound bed provides full surface adherence of grafts and skin flaps. Full surface adherence minimizes areas of dead space between the wound bed and applied tissues. Elimination of dead space prevents shear irritation upon movement as well as reduces the void space under the skin that can host fluid build-up.

10.2. Pharmacodynamics

Thrombin is a highly specific protease that transforms the fibrinogen contained in Sealer Protein (Human) into fibrin. Part of the thrombin is adsorbed by the fibrin, and any excess thrombin is inactivated by protease inhibitors in the blood.

Fibrinolysis Inhibitor, Aprotinin, is a polyvalent protease inhibitor that prevents premature degradation of fibrin. Free Aprotinin has a half-life ($t_{1/2}$) of approx. 0.82 and is eliminated by the kidney. Preclinical studies with different fibrin sealant preparations simulating the fibrinolytic activity generated by extracorporeal circulation in patients during cardiovascular surgery have shown that incorporation of Aprotinin in the product formulation increases resistance of the fibrin sealant clot to degradation in a fibrinolytic environment.

10.3. Pharmacokinetics

ARTISS is intended for local application only, therefore systemic exposure or distribution to other organs or tissues is not expected and pharmacokinetic studies were not conducted.

10.4. Immunogenicity

All therapeutic proteins have the potential for immunogenicity.

The detection of antibody formation is highly dependent on the sensitivity and specificity of the assay. Additionally, the observed incidence of antibody (including neutralizing antibody) positivity in an assay may be influenced by several factors including assay methodology, sample handling, timing of sample collection, concomitant medications, and underlying disease. For these reasons, comparison of incidence of antibodies in the studies described below with the incidences of antibodies in other studies or to other products may be misleading.

11. Storage, Stability, and Disposal

When stored at $\leq -20^{\circ}\text{C}$ ($\leq -4^{\circ}\text{F}$), ARTISS (Fibrin Sealant (Human), Slow Set), in pre-filled syringes, is stable until the expiry date indicated on the label.

Room Temperature Storage: Unopened pouches, thawed at room temperature, may be stored for up to 7 days at room temperature (15°C to 25°C) after removal from the freezer.

Part 2: Scientific Information

13. Pharmaceutical Information

Drug Substance

Non-proprietary name of the drug substance(s): Fibrin Sealant (Human), Slow Set

Chemical name: Human Fibrinogen

Human Factor XIII

Synthetic Aprotinin

Human Thrombin

Calcium Chloride

Molecular formula: Not applicable

Molecular mass: Human Fibrinogen: 340,000 g/mol

Human Factor XIII: 190,000 g/mol

Synthetic Aprotinin: 6,511.5 g/mol

Human Thrombin: 33,800 g/mol

Calcium Chloride: 147.01 g/mol

Structural formula: Not applicable

Physicochemical properties:

Solutions for Tissue Sealant

Deep-frozen: colorless to pale yellow, opalescent frozen solutions.

After defrosting: colorless to pale yellow liquids.

Product Characteristics:

Sealer Protein (Human) / Aprotinin

Sealer Protein (Human) is a sterile, non-pyrogenic, vapor-heated and solvent/detergent treated preparation made from pooled human plasma. Sealer Protein (Human) is provided as a finished frozen liquid Sealer Protein-Aprotinin Solution pre-filled into one side of a double-chamber syringe (chamber containing Sealer Protein -Aprotinin Solution is marked as "1").

The active ingredient in Sealer Protein (Human) component is fibrinogen. In addition, Factor XIII is co-purified with clottable protein from human plasma. No Factor XIII is added to the Sealer Protein (Human) manufacturing process, resulting in a Factor XIII level of 0.6-10 U/mL in the drug product. A Fibrinolysis Inhibitor, Aprotinin (Synthetic) is included in the Sealer Protein (Human) component to preclude premature fibrinolysis. To obtain Sealer Protein Concentrate (Human), cryoprecipitate derived from the plasma is dissolved in buffer solution, solvent/detergent treated, purified by precipitation and washing steps, vapor heat treated,

formulated, sterile filtered, concentrated under vacuum and frozen in pre-filled syringes.

Thrombin (Human) / Calcium Chloride

Thrombin (Human) is a sterile, non-pyrogenic, vapor-heated and solvent/detergent treated preparation made from pooled human plasma. Thrombin (Human) is provided as a finished frozen liquid Thrombin-Calcium Chloride Solution pre-filled into one side of a double-chamber syringe (chamber containing Thrombin-Calcium Chloride solution is marked as “2”).

The active ingredient human Thrombin is prepared from plasma through a series of separation and filtration steps followed by incubation of the solution with calcium chloride to activate prothrombin to thrombin. The solution subsequently undergoes ultra/diafiltration, vapor heat treatment, solvent/detergent treatment, purification by ion exchange chromatography, formulation, sterile filtration, filling and freezing in pre-filled syringes.

Viral Inactivation

ARTISS (Fibrin Sealant (Human), Slow Set) is made from human plasma. Products made from human plasma may contain infectious agents, such as viruses, that can cause disease. The risk that such products will transmit an infectious agent has been reduced by screening plasma donors for prior exposure to certain viruses, by testing for the presence of certain current virus infections, and by inactivating and removing certain viruses in the course of the manufacture.

Fibrin Sealant is a two-component biological sealant produced from pooled human plasma. As for all plasma products, the following measures are implemented to ensure the safety of the product from the potential presence of pathogenic viruses in human plasma:

- Donor selection
- Donation testing of single donations and also at the mini-pool and manufacturing pool level
- The use of PCR assay system (PCR) for release of plasma pools
- Effective virus inactivation/removal steps integrated into the manufacturing process including validation

The plasma safety precautions, and virus inactivation/removal steps taken during the manufacture of ARTISS are equivalent to those used for TISSEEL VH S/D 500 IU.

Each plasma donation is tested for infectious markers for human immunodeficiency virus, types 1 and 2 (HIV-1/-2), hepatitis C virus (HCV) and hepatitis B surface antigen (HbsAg) The criteria for release of each single plasma donation for further manufacturing are as follows:

- HIV-1 / HIV-2 antibody: non-reactive
- HbsAg: non-reactive
- HCV antibody: non-reactive

Each manufacturing plasma pool is tested and released for further manufacturing only when

- non-reactive for Human Immunodeficiency Virus (HIV), Hepatitis C Virus (HCV), Hepatitis A Virus (HAV) and Hepatitis B Virus (HBV) using Nucleic Acid Testing (NAT)
- Parvovirus B19 concentration not exceeding 104 IU / mL as measured by NAT

Plasma pool are tested using HIQ-PCR = Hyland Immuno Quality Assured Polymerase Chain Reaction. With the PCR method, in general 500 genome equivalents/mL of the above viruses can be determined reliably, with the actual sensitivity of HIQ-PCR being below that. Therefore, all pools which have been tested and evaluated as being positive lead to exclusion from further processing.

The manufacturing procedure for ARTISS includes processing steps designed to further reduce the risk of viral transmission. In particular, vapor heating and solvent/detergent treatment processes are included in the manufacturing of Sealer Protein Concentrate and Thrombin. In addition the reduction factors as associated with DEAE-Sephadex Batch Chromatography and Ion Exchange Chromatography of the Thrombin drug substance purification were investigated.

The virus reduction factors (expressed as log₁₀) of independent manufacturing steps were as follows for each of the viruses tested:

Table 10: Reduction Factors for Virus Removal and/or Inactivation

Sealer Protein Component						
Manufacturing Step	Mean Reduction Factors [log10] of Virus Tested*					
	HIV-1	HAV	BVDV	PRV	MMV	B19V
Early Manufacturing Steps	n.d.	n.d.	n.d.	n.d.	2.7*	3.4**
					2.3**	
Solvent/Detergent Treatment	>5.3	n.d.	>5.7	>5.9	n.d.	n.d.
Vapor Heat Treatment	>5.5	>5.6	>5.7	>6.7	1.2	1.0
Overall Reduction Factor (ORF)	>10.8	>5.6	>11.4	>12.6	3.5	3.3
Thrombin Component						
Manufacturing Step	Mean Reduction Factors [log10] of Virus Tested*					
	HIV-1	HAV	BVDV	PRV	MMV	B19V
Removal of Thrombin precursor protein from Cryosupernatant	3.2	1.5	1.8	2.5	1.2	1.7
Vapor Heat Treatment	>5.5	>4.9	>5.3	>6.7	1.0	>4
Solvent/Detergent Treatment	>5.3	n.d.	>5.5	>6.4	n.d.	n.d.
Ion Exchange Chromatography	n.d.	n.d.	n.d.	n.d.	3.6	n.d.
Overall Reduction Factor (ORF)	>14.0	>6.4	>12.6	>15.6	5.8	>5.7

n.d. = not determined

* The mean RF of all runs was calculated. E.g., when two runs were performed in study A and one run in study B for HIV-1, then the mean of the three RF's was calculated and listed in the table.

** As a conservative value for general and robust Parvovirus reduction capacity in steps 1 to 8, 2.3 logs were calculated from MMV and B19V reduction factors (omitting the higher B19V reduction factor). For calculation of and rationale behind this value, see

further above in the section where the corresponding study is discussed. For calculation of virus-specific overall reduction factors, however, only virus-specific individual reduction factors were considered.

HIV-1: Human immunodeficiency virus 1; **HAV:** Hepatitis A virus; **BVDV:** Bovine viral diarrhea virus, a model for Hepatitis C virus; **PRV:** Pseudorabies virus, a model for enveloped DNA viruses, among those Hepatitis B virus; **MMV:** Mice minute virus, a model for Human Parvovirus B19, **B19V:** Human Parvovirus B19.

14. Clinical Trials

Clinical trials were conducted to test the efficacy and safety of ARTISS (Fibrin Sealant (Human), Slow Set). The main active ingredients of both the frozen and freeze-dried formulations are identical in composition and consist of:

- Human Fibrinogen 91mg/ml
- Human Thrombin 4 IU/ml,
- Other ingredients: factor XIII, synthetic Aprotinin and Calcium chloride

The only difference between the formulation is that one is frozen, ready to use (Study 550201) vs. freeze-dried (Study 550703 & 550901)

Table 11: Summary of differences in formulation and preparation of Study 550201, 550703, and 550901

Study #	Formulation/ Preparation
550201	ARTISS formulation FS VH S/D 4 s-apr a 2-component fibrin sealant with 4 IU/mL human thrombin, vapor heated, solvent detergent treated, with synthetic aprotinin, and provided in a frozen, ready-to-use formulation
550703 and 550901	The ARTISS formulation FS VH S/D 4 s-apr, a 2-component fibrin sealant with 4 IU/mL human thrombin, vapor heated, solvent detergent treated, with synthetic aprotinin (s-apr), a fibrinolysis inhibitor, provided in a freeze-dried formulation.

14.1. Clinical Trials by Indication

Table 12: Summary of trial design and patient demographics for clinical trials in fixation of autologous skin grafts and tissue flaps and as adjunct to adhere tissue flaps in facial rhytidectomy

Study #	Study design	Dosage, route of administration and duration	Study subjects (n)	Mean age (Range)	Sex (%)
550201	Phase 3, prospective, multicenter, unblinded, randomized, noninferiority, clinical trial evaluated the safety and efficacy of ARTISS 1 provided in a frozen, ready-to-use formulation for use in adhering skin grafts and promoting wound healing in subjects with burn wounds.	<p>Each subject served as his/her own control for tested donor sites.</p> <p>Site 1 (Test site): ARTISS (0.02-0.04 ml/cm²) administered locally via spray application using TISSOMAT spray device (Baxter Healthcare Corporation, Westlake Village, CA) onto donor and recipient site immediately after excision prior to autologous sheet skin graft placement.</p> <p>Site 2 (Control): Staples placed parallel to seam of grafts abutting designated test area, including test site with staples</p>	127	30.8 yrs (1-62)	Female 43 (33.9%) Male: 84 (66.1%)

¹ FS VH S/D 4 s-apr, a two-component fibrin sealant with 4 IU/mL human thrombin, vapor heated, solvent detergent treated, with aprotinin

Study #	Study design	Dosage, route of administration and duration	Study subjects (n)	Mean age (Range)	Sex (%)
		<p>Duration: Interventions were administered intraoperatively</p>			
550703	Phase 2, multi-center, prospective, randomized, evaluator-blinded study, to evaluate efficacy and safety of the adjuvant use of ARTISS, provided in a freeze-dried formulation, as compared to sutures and/or staples alone, in subjects undergoing rhytidectomy.	<p>Each subject served as his/her own control</p> <p>Face Side 1 (Test site): ARTISS at a recommended dosing volume of 0.02 ml/cm² to 0.04 ml/cm² aerosolized application to the subcutaneous plane in both the neck and the face using a painting motion from side to side via EASYSpray propellant gas control device and Spray Set to aerosolize and apply the ARTISS followed by placement of a Jackson-Pratt drain and application of suture and/or staple.</p> <p>Face Side 2 (Control): The control side of the face received placement of a Jackson-Pratt drain and suture and/or staple.</p>	45	55.1 yrs (43-70)	Female: 42 (93.3%) Male: 3 (6.7%)

Study #	Study design	Dosage, route of administration and duration	Study subjects (n)	Mean age (Range)	Sex (%)
		<p>Duration: Interventions were administered intraoperatively</p>			
550901	Phase 3, prospective, controlled, randomized, subject-blinded, multicenter study to evaluate safety and efficacy of the adjuvant use of ARTISS 2 provided in a freeze-dried formulation, as compared to sutures and/or staples alone, in adhering tissues in subjects undergoing rhytidectomy.	<p>Each subject served as his/her own control.</p> <p>Face Side 1 (Test site): ARTISS was to be applied to 1 side of a subject's face at a recommended dosing volume of 0.02 mL/cm² to 0.04 mL/cm² administered via spray to the subcutaneous plane in both the neck and the face area using a "painting motion" from side to side, followed by placement of a flat 7 mm Blake Silicone drain at the side of the face and sutures and/or staples.</p>	75	54.4 yrs (40-71)	<p>Female: 71 (94.7%)</p> <p>Male: 4 (5.3%)</p>

² FS VH S/D 4 s-apr, a 2-component fibrin sealant with 4 IU/mL human thrombin, vapor heated, solvent detergent treated, with synthetic aprotinin (s-apr),

Study #	Study design	Dosage, route of administration and duration	Study subjects (n)	Mean age (Range)	Sex (%)
		<p>(DUPLOJECT Preparation and Application System and the EASYSRAY propellant gas control unit device and Spray Set were to be used to aerosolize and deliver the IP).</p> <p>Face Side 2 (Control): The control side of the face received placement of a Flat 7 mm Blake Silicone drain at the side of the face and sutures and/or staples</p> <p>Duration: Interventions were administered intraoperatively</p>			

Study 550201

ARTISS was investigated for fixation of split thickness sheet skin grafts in burn patients in a prospective, randomized, controlled, multicenter clinical study. The primary statistical analysis was used to test non-inferiority of ARTISS compared to staples with respect to complete wound closure at Day 28 after surgery. To assess the non-inferiority of success rate in wound closure with ARTISS as compared to that with staples, a one-sided 97.5% confidence interval

for the difference of correlated proportions was calculated. The non-inferiority margin was set at -10%.

Subjects ≤ 65 years of age (including pediatric subjects) with total burn wounds measuring $\leq 40\%$ total body surface area (TBSA) were eligible for treatment. Subjects with electrical or chemical burns were excluded. Eligible subjects were required to have deep partial thickness or full thickness wounds. Burn wounds on digits or genitalia were not eligible for designation as a test site.

A total of 138 subjects were randomized and treated at 13 study sites. All 138 subjects were treated at one test site with ARTISS and a separate test site with staples (control). Of the 138 treated subjects, 94 (68.1%) were male and 44 (31.9%) were female. The mean \pm SD age was 30.8 ± 17.6 years; 19 (13.8%) subjects were ≤ 6 years old, 21 (15.2%) subjects were 7 to 18 years old, and 98 (71.0%) were > 18 years old. The mean \pm SD estimated TBSA for all burn wounds was $13.6 \pm 9.2\%$. The mean \pm SD estimated TBSA requiring skin grafting was $8.0 \pm 6.9\%$. The mean \pm SD estimated TBSA for the ARTISS test sites was $1.7 \pm 0.8\%$ and for the stapled test sites was $1.7 \pm 0.7\%$. Burn wound thickness was classified as full thickness in 106 (76.8%) of the 138 treated subjects, and partial thickness in 32 (23.2%) subjects.

Study 550703

Study 550703 was a phase 2, multi-center, prospective, randomized, evaluator-blinded study, comparing the adjuvant use of ARTISS to sutures and/or staples (the control intervention) in subjects undergoing rhytidectomy. This was a split-face rhytidectomy study where 1 side of the face was to be treated with the investigational product as an adjuvant to the control intervention and the other side was to receive the control intervention only. In this way each subject was to serve as his/her own control. Allocation of the side of the face that was to receive ARTISS was determined according to a predefined randomization scheme. The postoperative follow-up period was planned for 14 days. Healthy male and female subjects between 18 and 75 years of age that were planned for rhytidectomy were eligible for participation in this study. A total of 45 subjects were randomized and treated at a total of 6 study sites. The number of subjects randomized at each study site ranged from 5 to 10, and no single study site randomized a majority of subjects. All randomized subjects completed the study. There were no subjects under 43 years old or older than 70 years old enrolled in the study, with 5 subjects 65 to 70 years old, inclusive.

The primary efficacy endpoint was the visual comparison of ecchymosis at Day 3 between the ARTISS-treated side of the face and the side of the face receiving the control intervention, as assessed by 5 independent blinded reviewers using standard digital photographs. The proportion of subjects whose side of the face treated with ARTISS was evaluated as having less ecchymosis than the side of the face that received the control intervention was to be compared to the proportion of subjects whose side of the face that received the control

intervention was evaluated as having less ecchymosis than the side of the face treated with ARTISS. These proportions were to be compared in a 2-sided McNemar's test of paired proportions at an alpha level of 5%.

A secondary endpoint was the total drainage at 24 hours following surgery for each side of the face, as assessed by the blinded reviewers.

Study 550901

Study 550901 was a Phase 3, prospective, controlled, randomized, subject-blinded, multicenter study to compare the adjuvant use of ARTISS to the control intervention in subjects undergoing rhytidectomy. This was a split-face rhytidectomy study where 1 side of the face was to be treated with the investigational product as an adjuvant to the control intervention and the other side was to receive the control intervention only. In this way each subject was to serve as his/her own control. Allocation of the side of the face that was to receive ARTISS was determined according to a predefined randomization scheme. The postoperative follow-up period was planned for 14 days. Subjects were 18-75 years old at the time of screening and had planned facial rhytidectomy; Subjects were excluded from the study if they were pregnant or lactating, or had undergone previous face-lift surgery.

A total of 75 subjects were randomized and treated at 7 study sites. The number of subjects randomized at each study site ranged from 7 to 12, with no single study site with a majority of subjects. All subjects completed the study. Of the 75 randomized subjects, 71 (94.7%) were females and 4 (5.3%) were males. Subject age was between 40 and 71 years old, inclusively, and 8 subjects were 65 years old or older (65-71).

The primary objective of this study was to evaluate the effect of ARTISS use on flap adherence in subjects undergoing rhytidectomy, as indicated by drainage volume; lower drainage volume indicated better flap adherence. The primary endpoint was the total drainage volume collected from each side of the face at 24 (± 4 hours) post-surgery.

The primary efficacy endpoint analysis was to be carried out on the Full Analysis Set. Total volume of drainage at post-surgery on each side of the face was summarized with descriptive statistics. To assess the difference in drainage volume between the 2 sides of the face, a 2-sided paired t-test was conducted.

14.2. Comparative Bioavailability Studies

Burns (grafts) - Study 550201:

Table 13: Result of Study # 550201 in fixation of autologous skin grafts ARTISS and tissue flaps for treatment of Burns (ITT population, N=127)

Primary Endpoints	ARTISS site % (n/N)	Control site (Staples) % (n/N)	Difference in % complete wound closure (ARTISS - Staples) (95% CI)
Non-inferiority of ARTISS versus staples with respect to complete wound closure* by Day 28, as assessed by blinded evaluators	43.3% (55/127)	37.0% (47/127)	6.3% (-2.9%; 15.5%)

* Complete Wound Closure: as full coverage of the wound with a contiguous layer of viable epithelium

ITT: Intent to Treat- all subjects with an observed primary endpoint for both face sides.

The lower limit of the 97.5% confidence interval of the difference in % complete wound closure by Day 28 between ARTISS and staples was -2.9%, which exceeded the predefined noninferiority margin of -10%.

Facial Rhytidectomy (flaps) - Studies 550703 and 550901:

Table 14: Study 550703 Primary Endpoint: Summary of Outcome of the Visual Comparisons of Ecchymosis Between Two Sides of Face as Assessed by a Majority of Blinded Reviewers on Postoperative Day 3 in Patients Undergoing Rhytidectomy ITT (N=37*)

% (n/N) of subjects with equal degree of ecchymosis on both sides of the face	% (n/N) of subjects with less ecchymosis at the ARTISS site (ARTISS and staples/sutures) %	% (n/N) of subjects with less ecchymosis at the control side of the face (staples/sutures alone)
13 (0.35)	7 (0.19)	17 (0.46)

* (N= 37) indicates the number of subjects with an outcome assigned by majority of reviewers (3 or more).

Table 15: ARTISS as adjunct to staples to adhere tissue flaps in facial rhytidectomy: Drainage Volume (mL) in the First 24 hours Following Facial Rhytidectomy with ARTISS followed by Staples, and Control (sutures/staples alone), (Results of Studies 550703 and 550901, Full Analysis Set)

Clinical Study	Mean ± SD Drainage (mL) ARTISS/Control Side of the Face	Mean ± SD Drainage (mL) Control Side of the Face	p-Value
Phase 2 (Study 550703) 45 subjects	11.5 ± 13.7	26.8 ± 24.0	< 0.0001
Phase 3 (Study 550901) 75 subjects	7.7 ± 7.4	20.0 ± 11.3	< 0.0001

15. Microbiology

No microbiological information is required for this drug product.

16. Non-Clinical Toxicology

The studies performed with TISSEEL containing 500 IU thrombin concentration confirm the safety profile of ARTISS (Fibrin Sealant (Human), Slow Set), as the low concentration of thrombin (4 IU) is not expected to cause any further toxicity than the 500 IU thrombin concentration.

General toxicology Histological studies are considered important given that TISSEEL / ARTISS are authorized for local use. Accordingly, histology has been performed on various species in tissues ranging from skin, vessels, nerves, tendons, organ tissue to bone.

Single-dose toxicity was studied through the subcutaneous injection of TISSEEL (frozen) and TISSEEL s-apr (frozen) in rats and rabbit at 5 ml/kg and no toxicity was found. Single-dose toxicity was also studied through the intravenous injection of Synthetic Aprotinin in mouse (doses: 100,000 & 500,000 & 1,500,000 KIU/kg) and rat (doses: 200,000 & 400,000 & 800,000 KIU/kg) and no toxicity was found.

Local tolerance studies using a subcutaneously implanted spongiosa block model were conducted in rats and rabbits with fibrin sealants diluted to a Thrombin concentration of 4 IU/mL. Subcutaneous application of 0.2ml/block of TISSEEL (frozen) and TISSEEL s-apr (frozen) indicated no systemic toxicity. The local tolerance of synthetic aprotinin after intravenous and paravenous application in rabbit was also tested with a dose of 0.2 ml/block and no toxicity was found.

Genotoxicity Genotoxicity of TISSEEL (frozen) was investigated using Escherichia coli where in vitro mutagenicity studies were conducted and TISSEEL (frozen) was found to be non-

mutagenic. Synthetic aprotinin was also tested for mutagenic activity using the AMES test on Salmonella typhimurium and was found to be non-mutagenic.

Carcinogenicity Long-term animal studies to evaluate the carcinogenic potential of TISSEEL has not been performed.

Reproductive and developmental toxicology Long-term animal studies to determine the effect of TISSEEL on fertility has not been performed.

Juvenile toxicity Long-term animal studies related to juvenile toxicity has not been performed.

Special toxicology Studies for cellular compatibility using cytotoxicity as an endpoint were conducted intravenously on human lung fibroblasts (dose 0.5 ml/well) for TISSEEL (frozen & lyophilized) and TISSEEL s-apr (frozen). No toxicity response was found by test and reference items. This was also performed for synthetic aprotinin intravenously on human lung fibroblasts and no toxicity response was found.

A skin sensitization study was performed on guinea pigs to detect the potential of synthetic aprotinin (doses: 0.1 ml, 0.3 ml & 0.5 ml). This was done intradermal and epicutan. No skin sensitizing potential of synthetic Aprotinin was shown in a Guinea Pig Maximization Test.

Patient Medication Information

READ THIS FOR SAFE AND EFFECTIVE USE OF YOUR MEDICINE

Pr ARTISS

Fibrin Sealant (Human), Slow Set

This patient medication information is written for the person who will be taking **ARTISS**. This may be you or a person you are caring for. Read this information carefully. Keep it as you may need to read it again.

This patient medication information is a summary. It will not tell you everything about this medication. If you have more questions about this medication or want more information about **ARTISS**, talk to a healthcare professional.

Serious warnings and precautions box

- ARTISS is for topical use only. ARTISS must not be injected inside a blood vessel because this may cause life-threatening blood clots.
- Risk of air getting into the blood circulation which can be serious or life-threatening
- Serious allergic (hypersensitive) reactions to any of the ingredients of ARTISS can occur. If you have any allergic reaction, your doctor will stop the use of ARTISS immediately and give you appropriate treatment.
- ARTISS is made from human blood which may carry a risk of transmitting infectious agents (e.g. viruses) that can cause disease.

What ARTISS is used for:

ARTISS is a tissue sealant.

- the fixation (gluing) of autologous skin grafts and tissue flaps.
- as an adjunct to haemostasis on subcutaneous tissue surfaces to treat burns in adult and pediatric patients.
- as an adjunct to adhere tissue flaps during facial rhytidectomy surgery (face-lift).

How ARTISS works:

ARTISS is a two-component fibrin sealant, and it contains two of the proteins that make blood clot. These proteins are called fibrinogen and thrombin. When these proteins mix during application, they form a clot where the surgeon applies them.

ARTISS is prepared as two solutions (Sealer Protein Solution and Thrombin Solution), which

mix when applied.

The ingredients in ARTISS are:

Medicinal ingredient(s): Sealer Protein-Aprotinin Solution & Thrombin-Calcium Chloride Solution

Non-medicinal ingredients: Nonmedicinal ingredients in the Sealer Protein-Aprotinin solution are human albumin, niacinamide and water for injection (WFI).

Nonmedicinal ingredients in the Thrombin-Calcium Chloride solution are human albumin, sodium chloride and water for injection (WFI). Sodium Hydroxide and Hydrochloric Acid are used to adjust the pH in both solutions.

ARTISS comes in the following dosage form(s):

2-, 4- and 10-mL pack sizes.

Do not use ARTISS if:

- you are allergic to any of the active substances or any other ingredients of this medicine (see “The ingredients in ARTISS are” above),
- you have a known hypersensitivity to Aprotinin

To help avoid side effects and ensure proper use, talk to your healthcare professional before you take ARTISS. Talk about any health conditions or problems you may have, including if you:

- are pregnant or breast-feeding
- have ever received ARTISS or aprotinin before, even if you did not have an allergic reaction to it. It is possible your body may have become sensitive to ARTISS, even if you did not react to the first application. If you think you have received either product in a previous operation, you have to inform your doctor about this.

Other warnings you should know about:

- ARTISS is made from human plasma and may carry a risk of transmitting infectious agents (e.g. viruses), despite manufacturing steps designed to reduce this risk. These steps include: using plasma obtained from the blood of healthy donors; testing of each plasma donation as well as the manufacturing plasma pools for certain viruses; a manufacturing process that has been shown to remove or inactivate some viruses and other pathogens.
- ARTISS MUST NOT be injected into blood vessels (veins or arteries), or into tissues. As ARTISS forms a clot where it is applied, injecting ARTISS may cause serious reactions (e.g., vessel occlusion blockage)
- ARTISS alone should not be used for the treatment of massive brisk arterial or venous severe or rapid bleeding from an artery or vein.

Tell your healthcare professional about all the medicines you take, including any drugs, vitamins, minerals, natural supplements or alternative medicines.

The following may [also] interact with ARTISS:

- ARTISS can be used when you are receiving other medical products. There are no known interactions between ARTISS and other medicinal products.

How to take ARTISS:

- ARTISS will be applied to you in a healthcare setting and only by an experienced surgeon who is been appropriately trained. ARTISS will be applied by dripping or spraying.

Usual dose:

The surgeon will determine the amount of ARTISS to use based on your needs during surgery.

Overdose:

As the product is actively used by the surgeon, overdose is very unlikely to occur. ARTISS (Fibrin Sealant (Human), Slow Set) is only to be used by a physician in a hospital setting.

Excessive thickness of the fibrin layer may interfere with the wound healing process.

If you think you, or a person you are caring for, have taken too much ARTISS, contact a healthcare professional, hospital emergency department, regional poison control centre or Health Canada's toll-free number, 1-844 POISON-X (1-844-764-7669) immediately, even if there are no signs or symptoms.

If you have any further questions on the use of this product, ask your doctor or pharmacist.

Possible side effects from using ARTISS:

These are not all the possible side effects you may have when taking ARTISS. If you experience any side effects not listed here, tell your healthcare professional.

The most common side effects with ARTISS are as follows:

- Itching
- Bruising at the site of the surgery
- Build-up of fluid under the skin at the site of the surgery
- Failure of the skin graft

Serious side effects and what to do about them

Frequency/Side Effect/Symptom	Talk to your healthcare professional		Stop taking the/this drug (if applicable) and get immediate medical help
	Only if severe	In all cases	
Severe allergic reactions: Skin rash, hives, chest tightness, wheezing, swelling of tongue or throat, light headedness, nausea, or vomiting		√	
Thromboembolic events/Air embolism: Shortness of breath, rapid breathing, chest pain, increased heart rate		√	

If you have a troublesome symptom or side effect that is not listed here or becomes bad enough to interfere with your daily activities, tell your healthcare professional.

Reporting side effects

You can report any suspected side effects associated with the use of health products to Health Canada by:

- Visiting the Web page on Adverse Reaction Reporting (canada.ca/drug-device-reporting) for information on how to report online, by mail or by fax; or
- Calling toll-free at 1-866-234-2345.

NOTE: Contact your healthcare professional if you need information about how to manage your side effects. The Canada Vigilance Program does not provide medical advice.

Storage:

Keep out of reach and sight of children.

Keep the syringe in the outer carton in order to protect from light.

Do not use this medicine after the expiry date which is stated on the label after “EXP”.

Store and transport frozen (at $\leq -20^{\circ}\text{C}$). The cold storage chain must not be interrupted until use.

Storage after thawing:

After thawing, the solutions must not be refrozen or refrigerated. Unopened pouches, thawed at room temperature, may be stored for up to 7 days at controlled room temperature (15°C to

25°C).

The product must be used within 12 hours after warming to 33°C to 37°C or removal from original pouches.

If you want more information about ARTISS:

- Talk to your healthcare professional
- Find the full product monograph that is prepared for healthcare professionals and includes the Patient Medication Information by visiting the Health Canada Drug Product Database website (<https://www.canada.ca/en/health-canada/services/drugs-health-products/drug-products/drug-product-database.html>); the manufacturer's website www.baxter.ca or by calling 1-888-719-9955.

Date of Authorization: 2025-09-03